

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021925\  
 Data File : BF141675.D  
 Acq On : 19 Feb 2025 15:16  
 Operator : RC/JU  
 Sample : Q1382-03  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 OU4-PCS-TC-02-021725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141675.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 4.998       | 489           | 494         | 513          | rVB      | 16604          | 30534         | 1.26%           | 0.187%        |
| 2         | 5.404       | 557           | 563         | 587          | rBV      | 1512677        | 2075009       | 85.91%          | 12.675%       |
| 3         | 6.422       | 730           | 736         | 765          | rBV      | 1496123        | 2120779       | 87.80%          | 12.954%       |
| 4         | 6.781       | 791           | 797         | 805          | rBV      | 434801         | 554359        | 22.95%          | 3.386%        |
| 5         | 7.345       | 886           | 893         | 904          | rBV      | 966802         | 1358873       | 56.26%          | 8.300%        |
| 6         | 7.604       | 932           | 937         | 955          | rBV      | 23085          | 44883         | 1.86%           | 0.274%        |
| 7         | 8.063       | 1009          | 1015        | 1035         | rBV      | 529362         | 744145        | 30.81%          | 4.545%        |
| 8         | 9.134       | 1191          | 1197        | 1208         | rBV      | 1778295        | 2353914       | 97.45%          | 14.379%       |
| 9         | 9.810       | 1307          | 1312        | 1328         | rBV      | 606106         | 833377        | 34.50%          | 5.091%        |
| 10        | 10.528      | 1429          | 1434        | 1441         | rBV      | 128906         | 163617        | 6.77%           | 0.999%        |
| 11        | 10.604      | 1441          | 1447        | 1463         | rBV      | 1132544        | 1513450       | 62.66%          | 9.245%        |
| 12        | 11.298      | 1560          | 1565        | 1574         | rBV      | 630406         | 829104        | 34.33%          | 5.064%        |
| 13        | 11.827      | 1650          | 1655        | 1678         | rBV      | 122760         | 256101        | 10.60%          | 1.564%        |
| 14        | 12.616      | 1784          | 1789        | 1800         | rBV4     | 12970          | 37468         | 1.55%           | 0.229%        |
| 15        | 12.880      | 1829          | 1834        | 1848         | rVB      | 1803202        | 2415411       | 100.00%         | 14.754%       |
| 16        | 13.786      | 1983          | 1988        | 2003         | rBV9     | 12906          | 48589         | 2.01%           | 0.297%        |
| 17        | 13.939      | 2008          | 2014        | 2025         | rVB      | 406403         | 568443        | 23.53%          | 3.472%        |
| 18        | 15.380      | 2253          | 2259        | 2272         | rBV      | 251667         | 422986        | 17.51%          | 2.584%        |




Sum of corrected areas: 16371042

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021925\  
Data File : BF141675.D  
Acq On : 19 Feb 2025 15:16  
Operator : RC/JU  
Sample : Q1382-03  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
OU4-PCS-TC-02-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

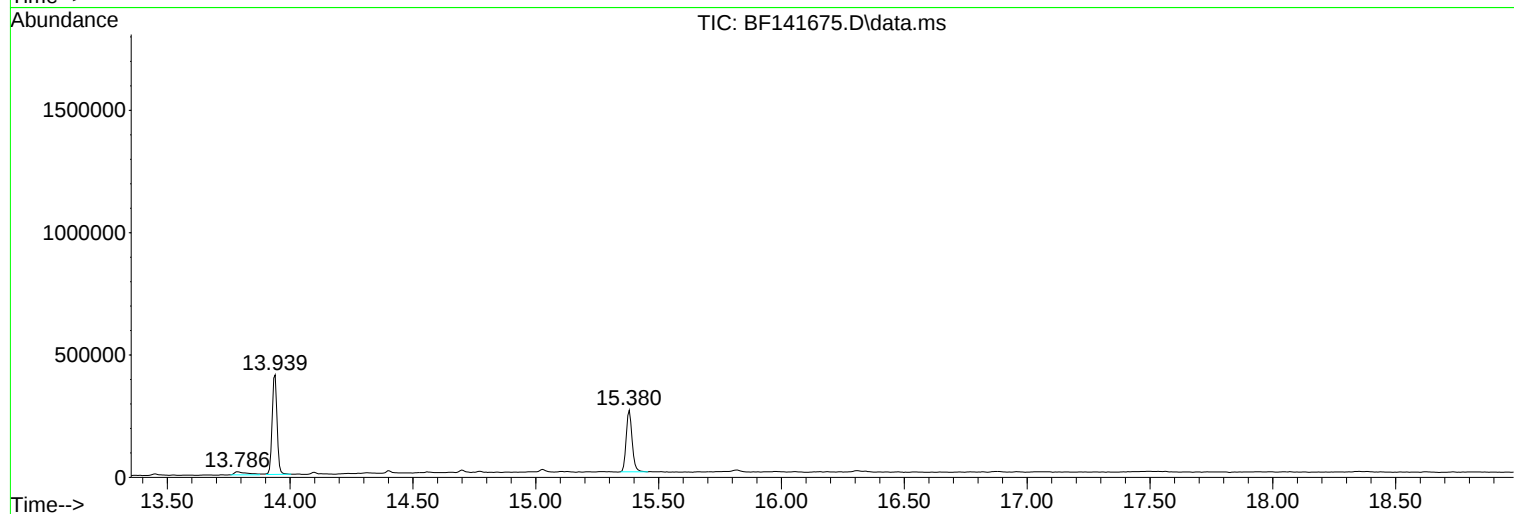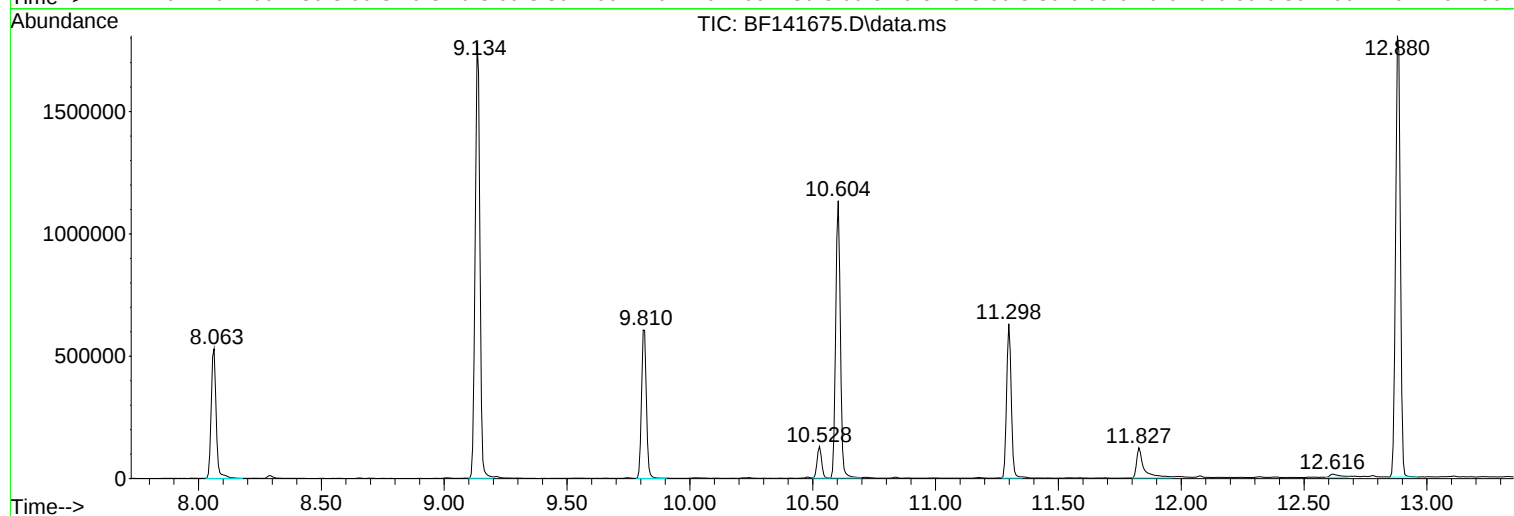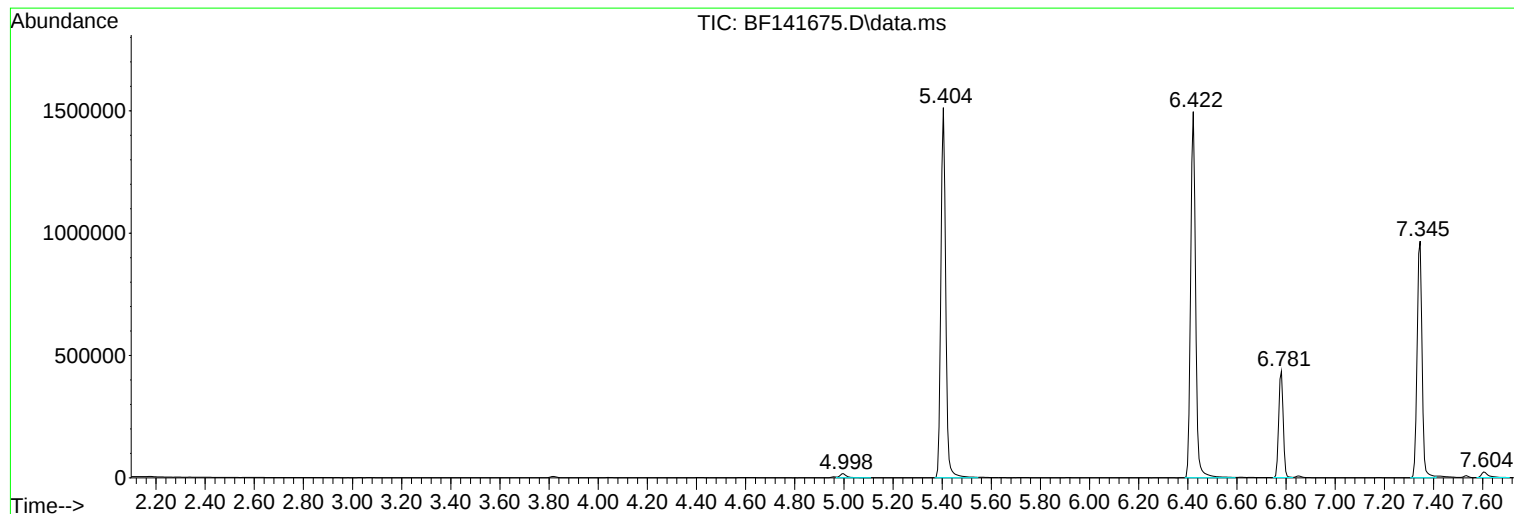

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021925\  
Data File : BF141675.D  
Acq On : 19 Feb 2025 15:16  
Operator : RC/JU  
Sample : Q1382-03  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
OU4-PCS-TC-02-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021925\  
Data File : BF141675.D  
Acq On : 19 Feb 2025 15:16  
Operator : RC/JU  
Sample : Q1382-03  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
OU4-PCS-TC-02-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|