

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
 Data File : BF141676.D
 Acq On : 19 Feb 2025 15:45
 Operator : RC/JU
 Sample : Q1382-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-TC-03-021725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141676.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.993	489	493	511	rVB	15498	28308	1.27%	0.199%
2	5.404	557	563	589	rBV	1288081	1790532	80.58%	12.577%
3	6.422	730	736	762	rBV	1294749	1843400	82.96%	12.949%
4	6.781	792	797	805	rBV	407106	513440	23.11%	3.607%
5	7.345	887	893	905	rBV	831428	1173383	52.80%	8.242%
6	7.610	931	938	959	rBV	19097	46502	2.09%	0.327%
7	8.063	1009	1015	1033	rBV	485396	678459	30.53%	4.766%
8	9.133	1192	1197	1208	rBV	1688937	2222138	100.00%	15.609%
9	9.816	1307	1313	1327	rBV	554596	760838	34.24%	5.344%
10	10.528	1429	1434	1441	rBV	186404	241203	10.85%	1.694%
11	10.604	1441	1447	1463	rVV	960975	1294849	58.27%	9.095%
12	11.298	1560	1565	1582	rBV	541290	732704	32.97%	5.147%
13	11.827	1650	1655	1677	rBV	51580	125301	5.64%	0.880%
14	12.880	1828	1834	1847	rBV	1511556	1953131	87.89%	13.719%
15	13.933	2008	2013	2024	rVB	296887	430257	19.36%	3.022%
16	15.380	2253	2259	2271	rBV	236244	401821	18.08%	2.823%




Sum of corrected areas: 14236266

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141676.D
Acq On : 19 Feb 2025 15:45
Operator : RC/JU
Sample : Q1382-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-03-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

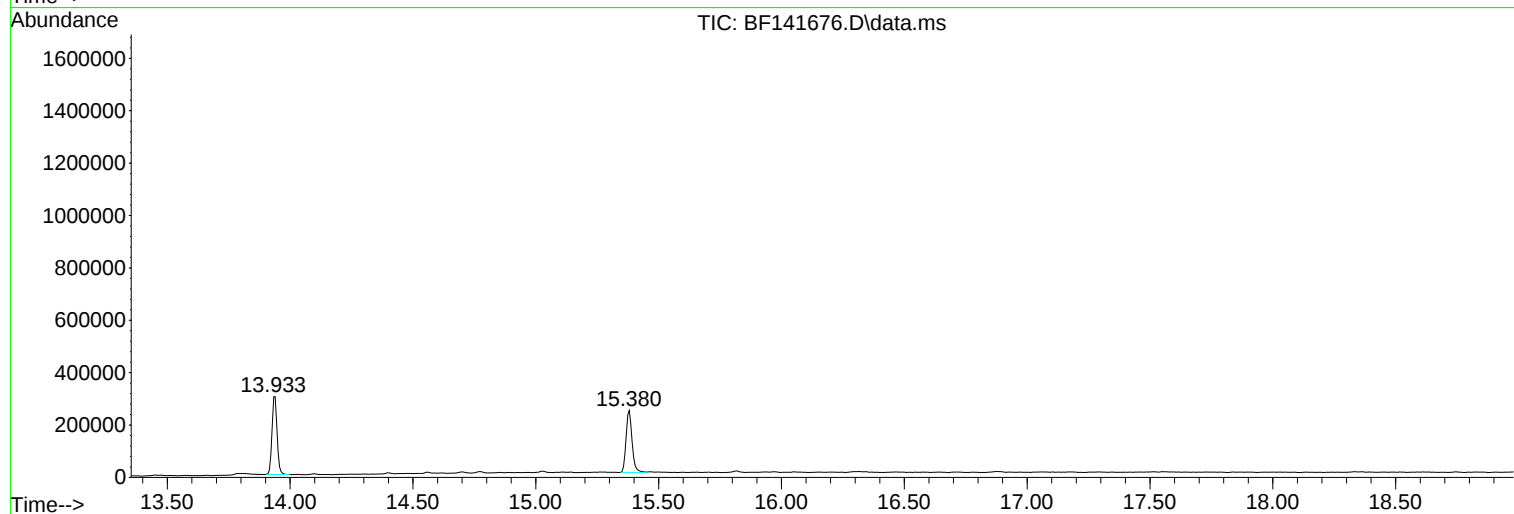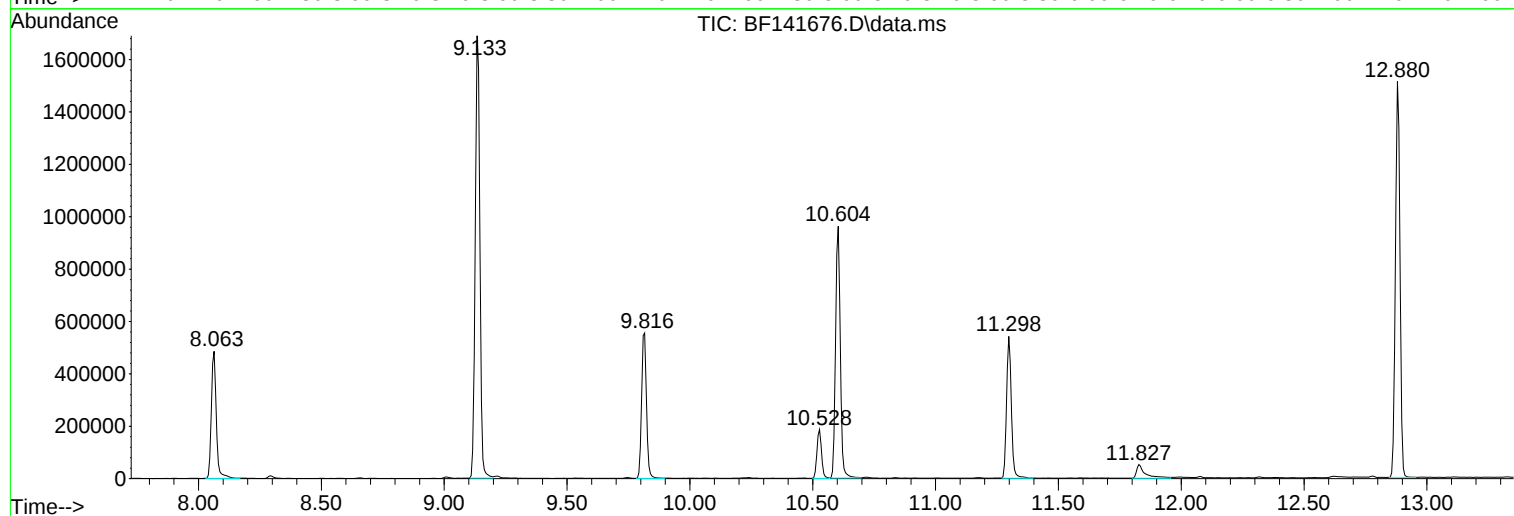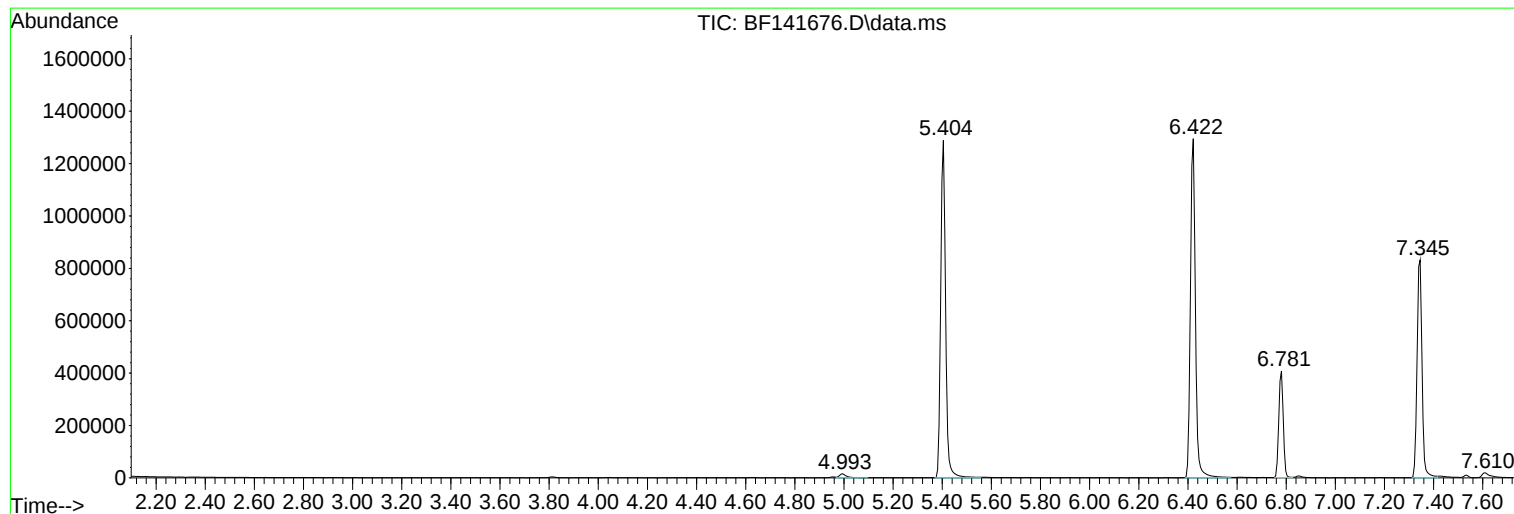

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141676.D
Acq On : 19 Feb 2025 15:45
Operator : RC/JU
Sample : Q1382-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-03-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141676.D
Acq On : 19 Feb 2025 15:45
Operator : RC/JU
Sample : Q1382-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-03-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------