

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
 Data File : BF141680.D
 Acq On : 19 Feb 2025 17:43
 Operator : RC/JU
 Sample : Q1382-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-TC-05-021725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141680.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.998	490	494	506	rVB	18921	30726	1.16%	0.190%
2	5.404	557	563	587	rBV	1562198	2135340	80.38%	13.193%
3	6.422	730	736	764	rBV	1544638	2184850	82.24%	13.499%
4	6.781	792	797	805	rBV	405360	510771	19.23%	3.156%
5	7.345	887	893	904	rBV	1037313	1434376	53.99%	8.862%
6	7.610	933	938	955	rVB	18434	43737	1.65%	0.270%
7	8.063	1009	1015	1021	rBV	497754	670407	25.24%	4.142%
8	9.133	1191	1197	1209	rBV	2001956	2656652	100.00%	16.414%
9	9.810	1307	1312	1325	rBV	553638	763212	28.73%	4.715%
10	10.528	1429	1434	1441	rBV	126811	162742	6.13%	1.005%
11	10.604	1441	1447	1463	rBV	1107903	1503947	56.61%	9.292%
12	11.298	1560	1565	1580	rVB	549771	741116	27.90%	4.579%
13	11.827	1650	1655	1673	rBV2	72402	151980	5.72%	0.939%
14	12.880	1828	1834	1845	rBV	1805202	2371082	89.25%	14.650%
15	13.933	2008	2013	2023	rVB	299457	430147	16.19%	2.658%
16	15.380	2253	2259	2271	rBV	234485	394314	14.84%	2.436%




Sum of corrected areas: 16185399

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141680.D
Acq On : 19 Feb 2025 17:43
Operator : RC/JU
Sample : Q1382-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-05-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

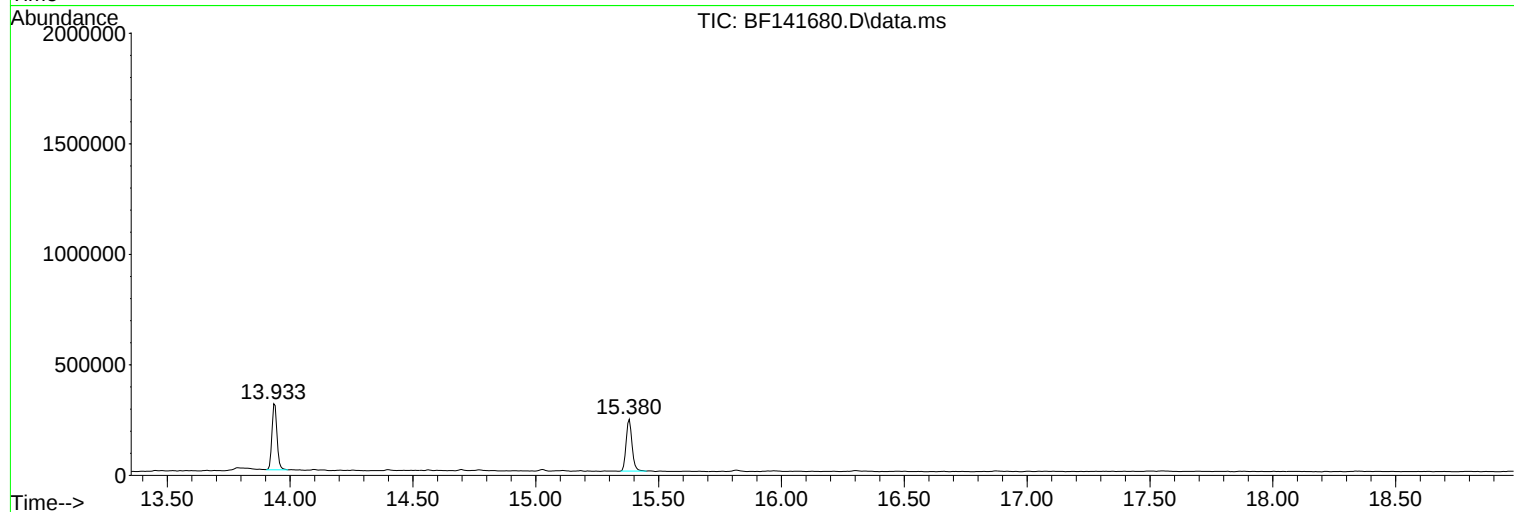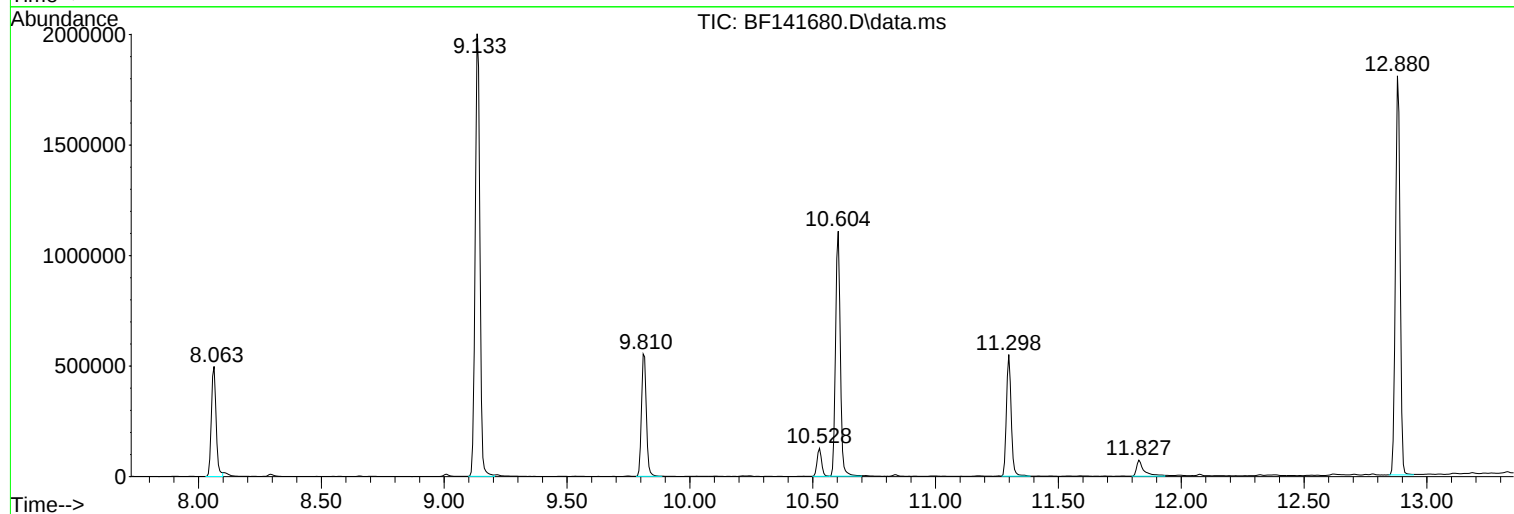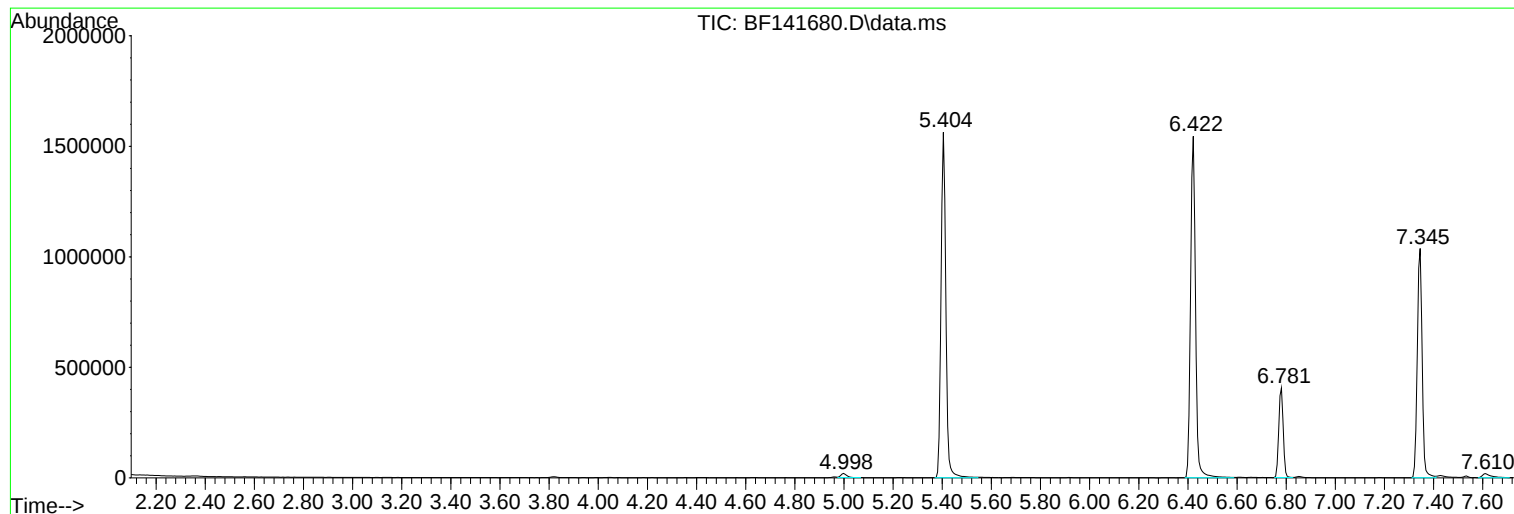

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141680.D
Acq On : 19 Feb 2025 17:43
Operator : RC/JU
Sample : Q1382-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-05-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141680.D
Acq On : 19 Feb 2025 17:43
Operator : RC/JU
Sample : Q1382-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-05-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------