

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021925\  
 Data File : BF141683.D  
 Acq On : 19 Feb 2025 19:11  
 Operator : RC/JU  
 Sample : Q1382-15  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 OU4-PCS-TC-08-021725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141683.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.404       | 557           | 563         | 580          | rBV      | 1052255        | 1530583       | 81.32%          | 12.001%       |
| 2         | 6.416       | 730           | 735         | 761          | rBV      | 1086255        | 1582596       | 84.08%          | 12.408%       |
| 3         | 6.781       | 792           | 797         | 805          | rBV      | 409072         | 522522        | 27.76%          | 4.097%        |
| 4         | 7.345       | 887           | 893         | 905          | rBV      | 706646         | 1006457       | 53.47%          | 7.891%        |
| 5         | 7.616       | 933           | 939         | 956          | rVB3     | 9549           | 29289         | 1.56%           | 0.230%        |
| 6         | 8.063       | 1009          | 1015        | 1034         | rBV      | 492844         | 694183        | 36.88%          | 5.443%        |
| 7         | 9.133       | 1192          | 1197        | 1208         | rBV      | 1455764        | 1882172       | 100.00%         | 14.757%       |
| 8         | 9.810       | 1307          | 1312        | 1327         | rBV      | 566060         | 785091        | 41.71%          | 6.156%        |
| 9         | 10.528      | 1429          | 1434        | 1441         | rBV      | 161056         | 214409        | 11.39%          | 1.681%        |
| 10        | 10.604      | 1441          | 1447        | 1464         | rVV      | 744480         | 1050339       | 55.80%          | 8.235%        |
| 11        | 11.298      | 1560          | 1565        | 1581         | rBV      | 572659         | 771325        | 40.98%          | 6.048%        |
| 12        | 11.827      | 1650          | 1655        | 1674         | rBV3     | 21838          | 54116         | 2.88%           | 0.424%        |
| 13        | 12.880      | 1828          | 1834        | 1843         | rBV      | 1365242        | 1745015       | 92.71%          | 13.682%       |
| 14        | 13.933      | 2008          | 2013        | 2027         | rVB      | 312490         | 456423        | 24.25%          | 3.579%        |
| 15        | 15.380      | 2252          | 2259        | 2273         | rBV      | 248638         | 429676        | 22.83%          | 3.369%        |




Sum of corrected areas: 12754196

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021925\  
Data File : BF141683.D  
Acq On : 19 Feb 2025 19:11  
Operator : RC/JU  
Sample : Q1382-15  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
OU4-PCS-TC-08-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

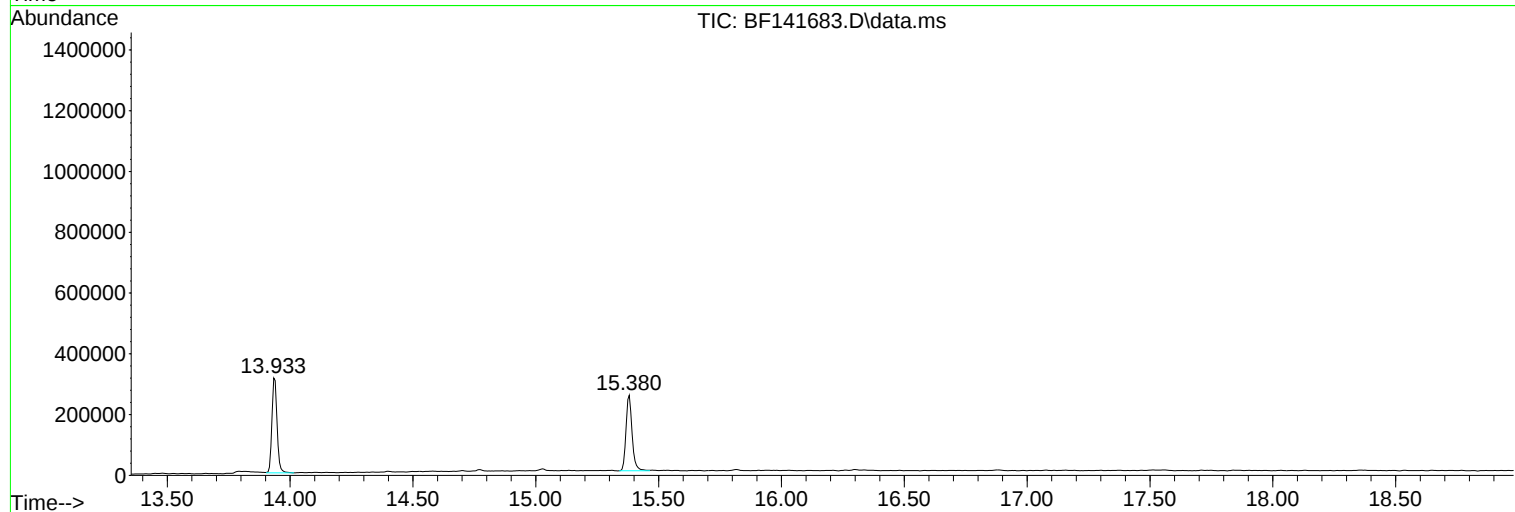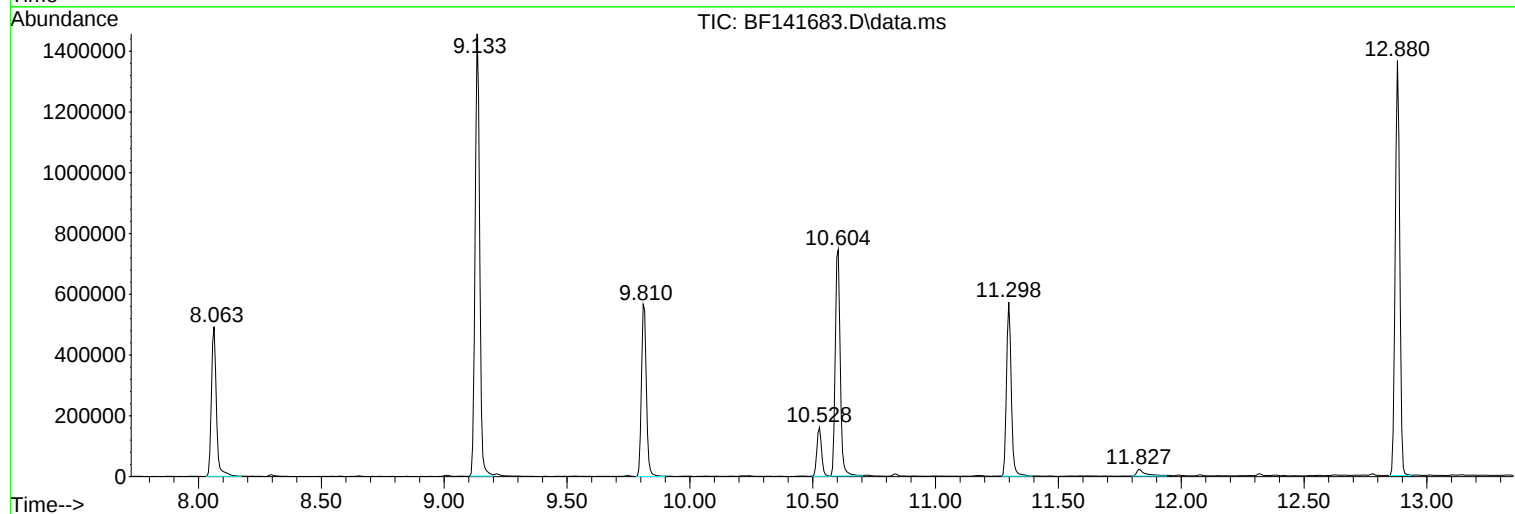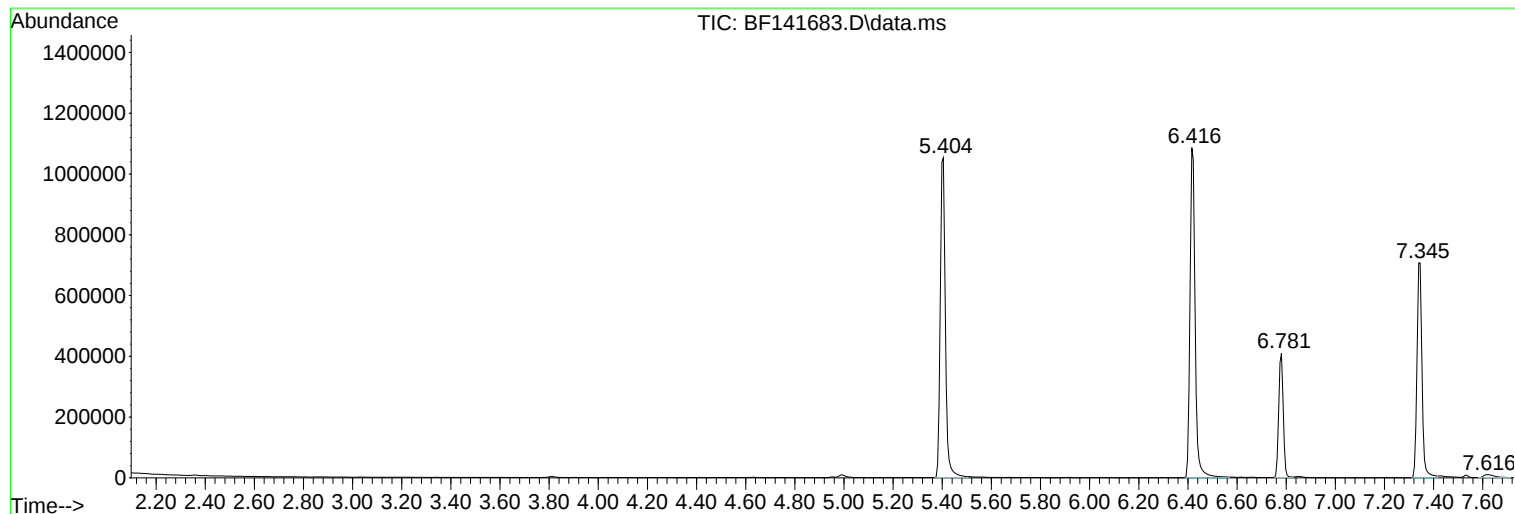

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021925\  
Data File : BF141683.D  
Acq On : 19 Feb 2025 19:11  
Operator : RC/JU  
Sample : Q1382-15  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
OU4-PCS-TC-08-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021925\  
Data File : BF141683.D  
Acq On : 19 Feb 2025 19:11  
Operator : RC/JU  
Sample : Q1382-15  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
OU4-PCS-TC-08-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|