

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
 Data File : BF141684.D
 Acq On : 19 Feb 2025 19:41
 Operator : RC/JU
 Sample : Q1382-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-TC-09-021725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141684.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.993	489	493	504	rVB	11874	21024	1.07%	0.159%
2	5.404	557	563	599	rBV	1109137	1605056	81.34%	12.126%
3	6.416	730	735	764	rBV	1128976	1649859	83.61%	12.464%
4	6.781	792	797	804	rBV	416133	535962	27.16%	4.049%
5	7.340	887	892	905	rBV	729208	1045855	53.00%	7.901%
6	7.616	934	939	950	rBV2	11693	32573	1.65%	0.246%
7	8.063	1009	1015	1038	rBV	497403	714305	36.20%	5.396%
8	9.134	1192	1197	1208	rBV	1521151	1973189	100.00%	14.907%
9	9.810	1307	1312	1334	rVB	577965	804544	40.77%	6.078%
10	10.528	1429	1434	1441	rBV	196280	257455	13.05%	1.945%
11	10.604	1441	1447	1463	rVV	783455	1083138	54.89%	8.183%
12	11.298	1560	1565	1581	rBV	570484	782505	39.66%	5.912%
13	11.833	1650	1656	1668	rBV4	14641	37466	1.90%	0.283%
14	12.880	1828	1834	1843	rBV	1410088	1812635	91.86%	13.694%
15	13.939	2008	2014	2024	rVB	309738	450492	22.83%	3.403%
16	15.380	2253	2259	2271	rBV	250844	430702	21.83%	3.254%




Sum of corrected areas: 13236760

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141684.D
Acq On : 19 Feb 2025 19:41
Operator : RC/JU
Sample : Q1382-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-09-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

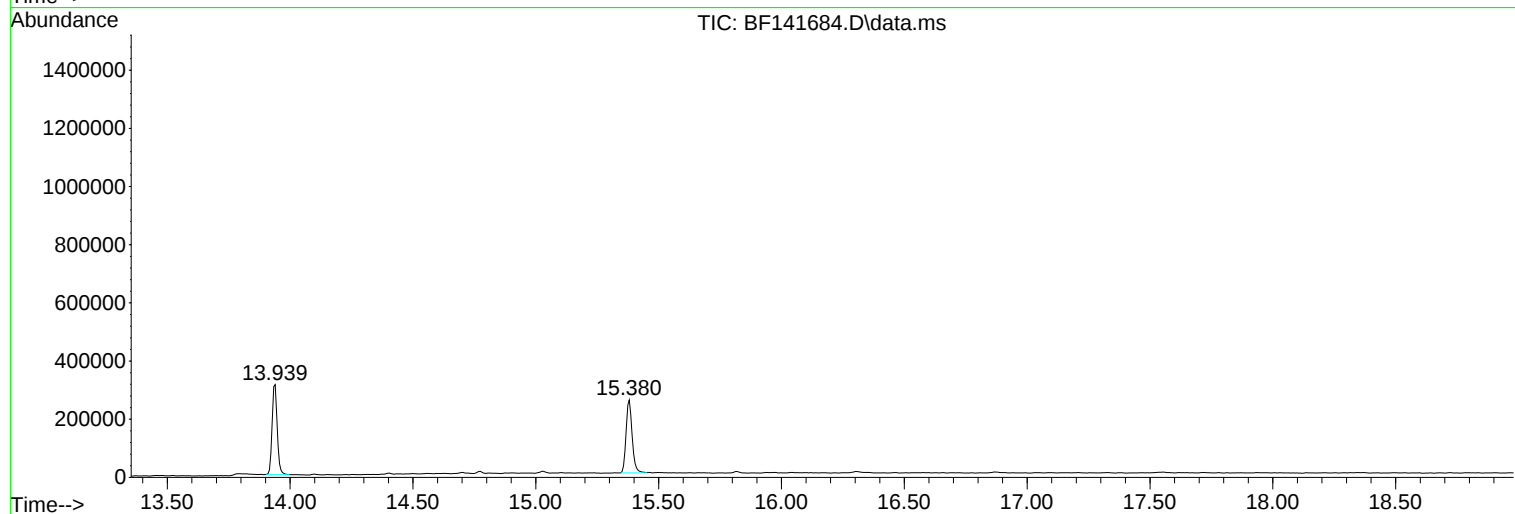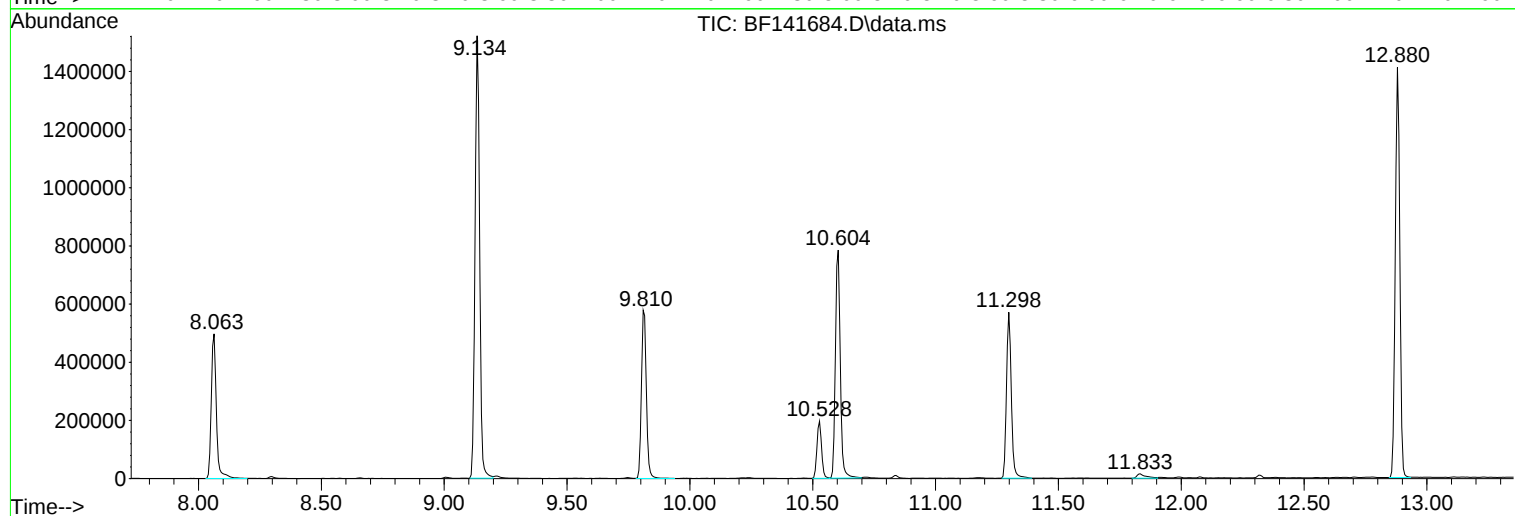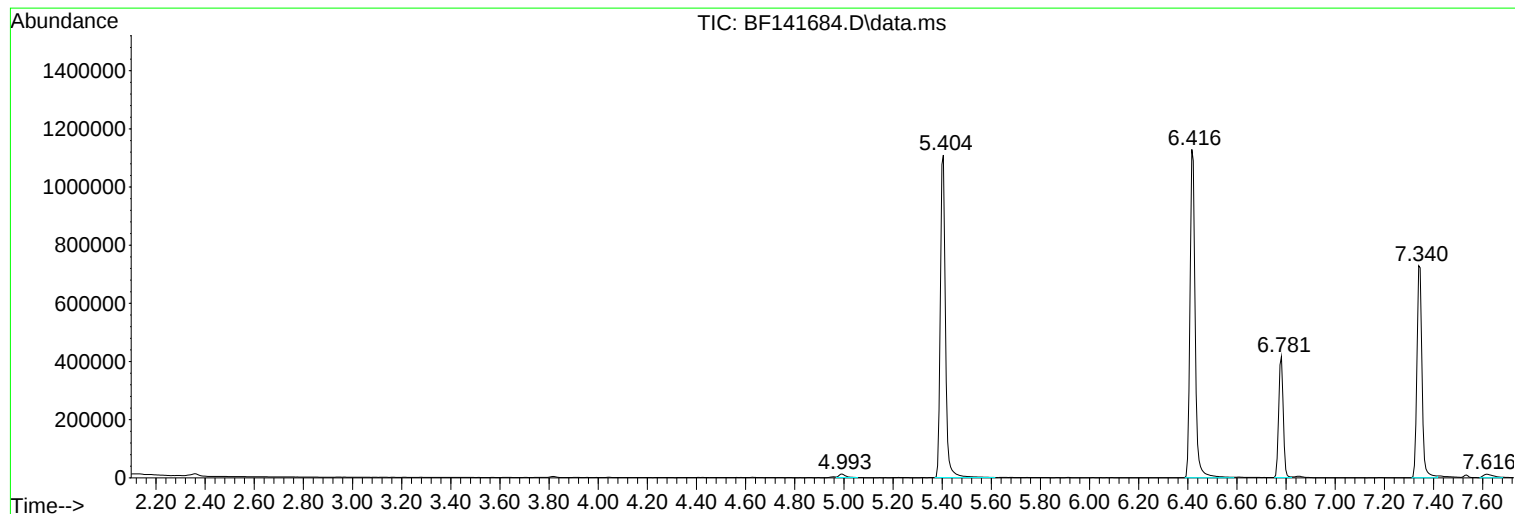

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141684.D
Acq On : 19 Feb 2025 19:41
Operator : RC/JU
Sample : Q1382-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-09-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141684.D
Acq On : 19 Feb 2025 19:41
Operator : RC/JU
Sample : Q1382-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-09-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
