

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
 Data File : BF141685.D
 Acq On : 19 Feb 2025 20:10
 Operator : RC/JU
 Sample : Q1382-19
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-TC-10-021725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141685.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.993	489	493	510	rVB	14068	26602	1.31%	0.198%
2	5.404	557	563	586	rBV	1126207	1622780	79.63%	12.076%
3	6.416	730	735	761	rBV	1178366	1690021	82.93%	12.577%
4	6.781	792	797	805	rBV	403519	526960	25.86%	3.922%
5	7.340	887	892	904	rBV	764961	1079241	52.96%	8.032%
6	7.616	933	939	955	rBV	12634	34820	1.71%	0.259%
7	8.063	1009	1015	1041	rBV	496892	708523	34.77%	5.273%
8	9.134	1192	1197	1208	rBV	1576987	2038003	100.00%	15.167%
9	9.810	1307	1312	1327	rBV	571219	777421	38.15%	5.785%
10	10.528	1429	1434	1441	rBV	200926	263255	12.92%	1.959%
11	10.604	1441	1447	1461	rVV	805983	1123871	55.15%	8.364%
12	11.298	1560	1565	1581	rVB	560702	764297	37.50%	5.688%
13	11.828	1650	1655	1674	rBV	46538	106349	5.22%	0.791%
14	12.880	1828	1834	1847	rBV	1421035	1807286	88.68%	13.450%
15	13.933	2008	2013	2024	rVB	309713	436465	21.42%	3.248%
16	15.380	2252	2259	2268	rBV	250331	431609	21.18%	3.212%




Sum of corrected areas: 13437503

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141685.D
Acq On : 19 Feb 2025 20:10
Operator : RC/JU
Sample : Q1382-19
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-10-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

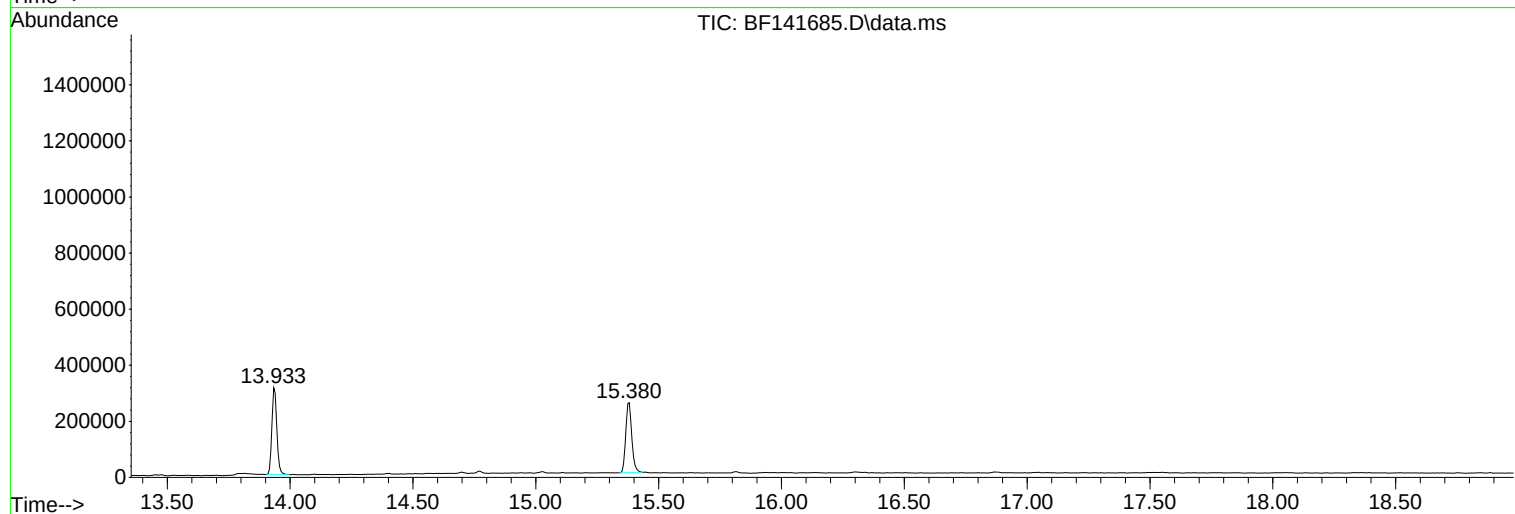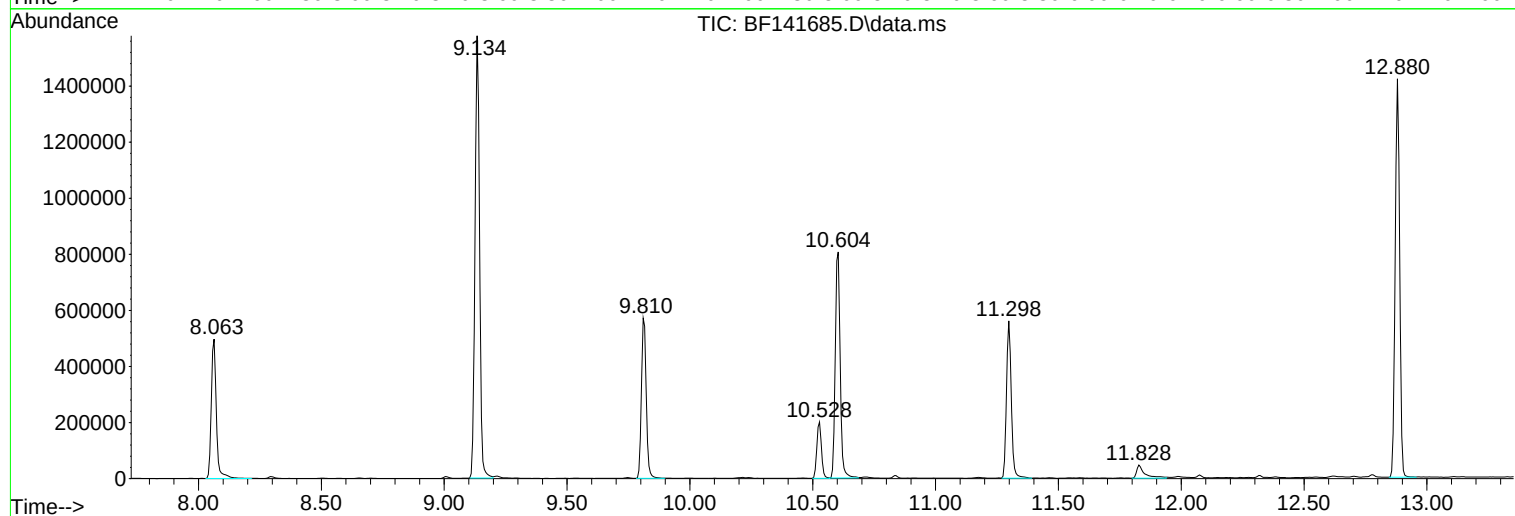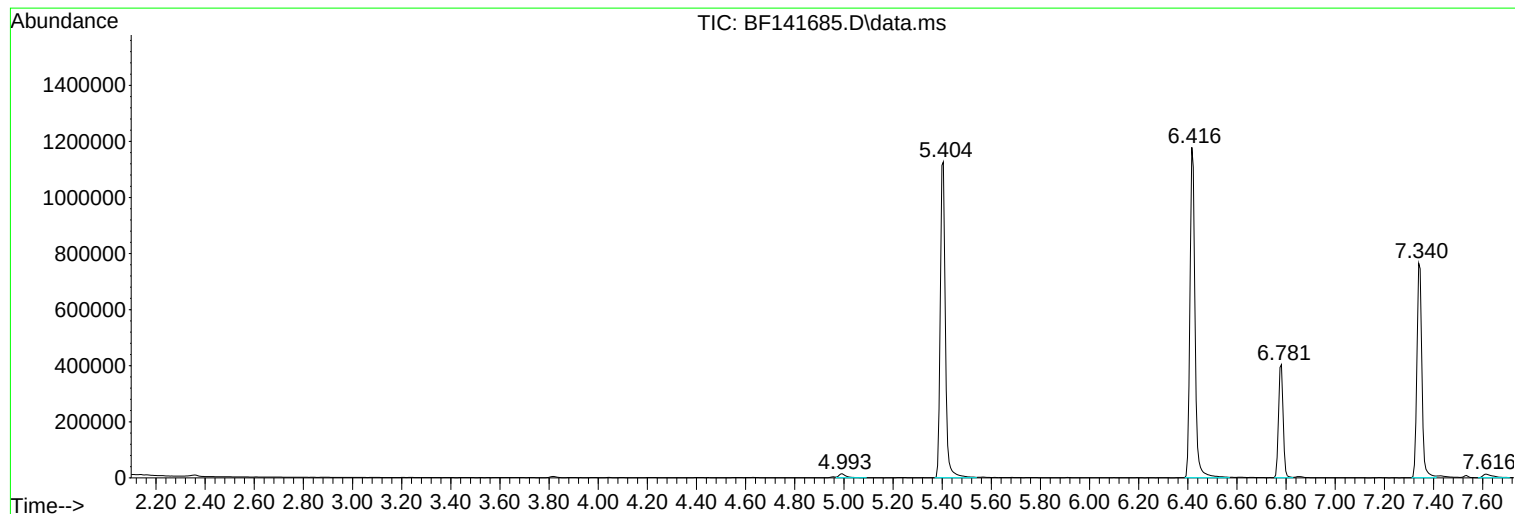

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141685.D
Acq On : 19 Feb 2025 20:10
Operator : RC/JU
Sample : Q1382-19
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-10-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141685.D
Acq On : 19 Feb 2025 20:10
Operator : RC/JU
Sample : Q1382-19
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-10-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------