

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
 Data File : BF141686.D
 Acq On : 19 Feb 2025 20:39
 Operator : RC/JU
 Sample : Q1383-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-TC-11-021725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141686.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.404	557	563	587	rBV	1176160	1660890	77.08%	12.204%
2	6.416	730	735	763	rBV	1176469	1693077	78.58%	12.440%
3	6.781	791	797	805	rBV	409859	528005	24.50%	3.880%
4	7.339	887	892	905	rBV	774359	1095433	50.84%	8.049%
5	7.610	933	938	950	rBV2	11703	32053	1.49%	0.236%
6	8.063	1009	1015	1033	rBV	495452	707583	32.84%	5.199%
7	9.004	1170	1175	1185	rBV	47090	66481	3.09%	0.488%
8	9.133	1190	1197	1215	rVV	1613695	2154703	100.00%	15.832%
9	9.810	1307	1312	1329	rBV	577894	793400	36.82%	5.830%
10	10.528	1429	1434	1441	rBV	242786	309771	14.38%	2.276%
11	10.604	1441	1447	1463	rVV	826739	1129409	52.42%	8.298%
12	11.298	1560	1565	1583	rVB	566078	773632	35.90%	5.684%
13	11.827	1650	1655	1659	rBV2	17447	30210	1.40%	0.222%
14	12.880	1828	1834	1842	rBV	1368391	1735478	80.54%	12.752%
15	13.933	2008	2013	2024	rVB	309490	444826	20.64%	3.268%
16	15.380	2252	2259	2274	rBV	259841	454933	21.11%	3.343%




Sum of corrected areas: 13609884

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141686.D
Acq On : 19 Feb 2025 20:39
Operator : RC/JU
Sample : Q1383-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-11-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

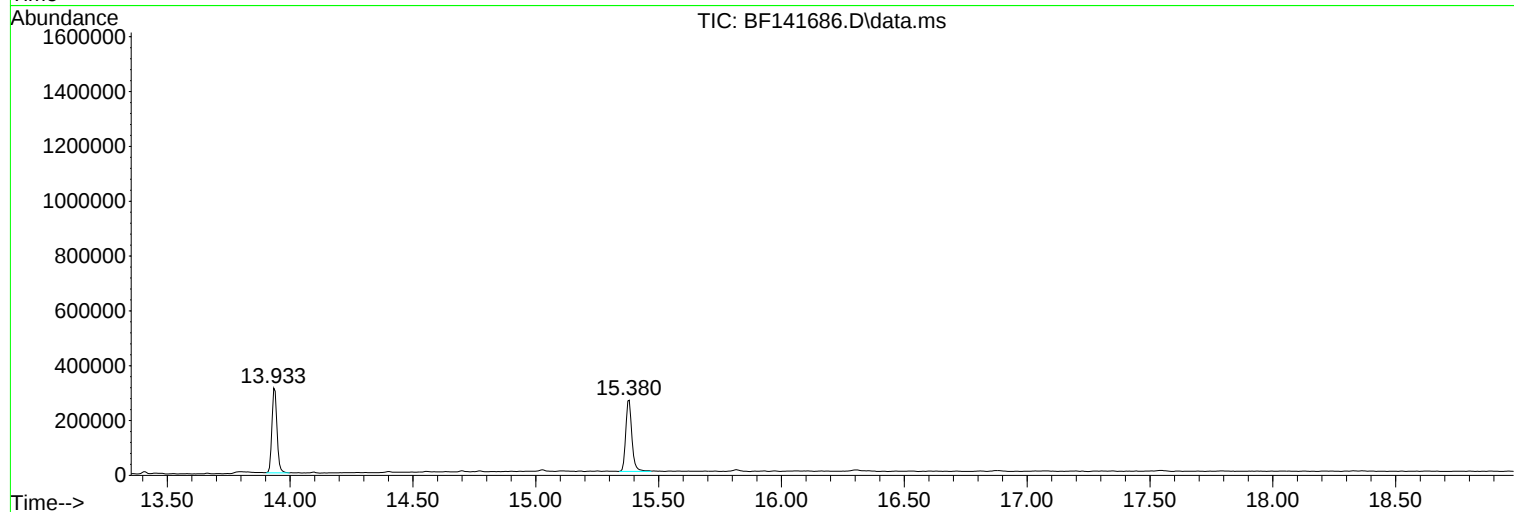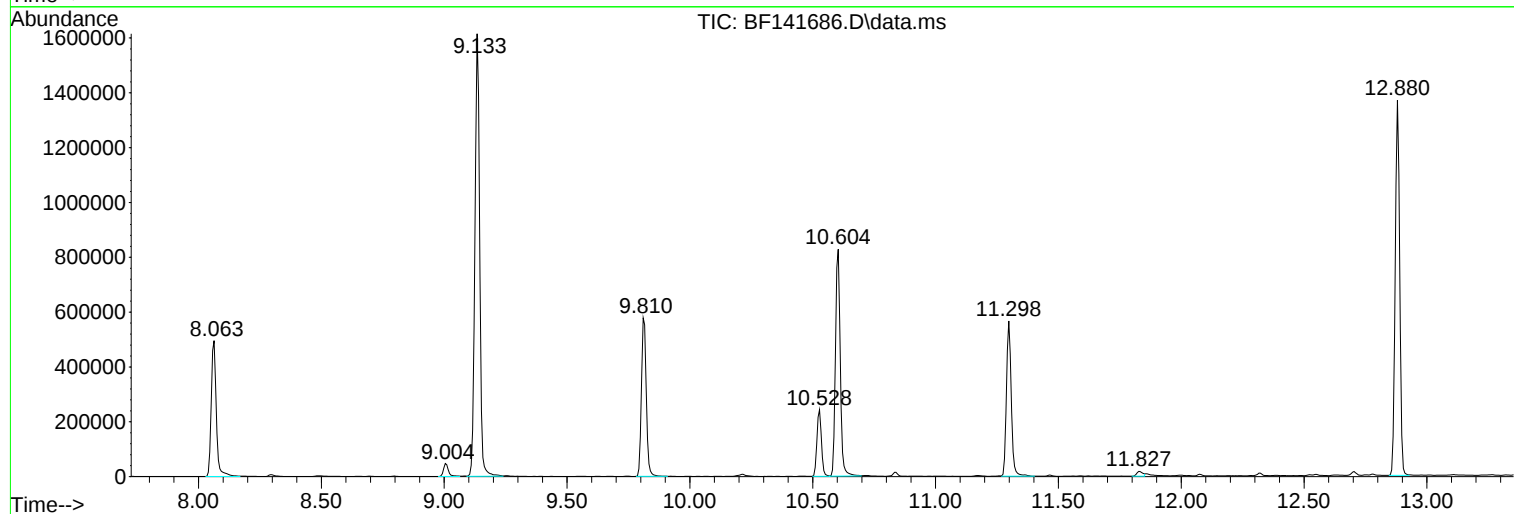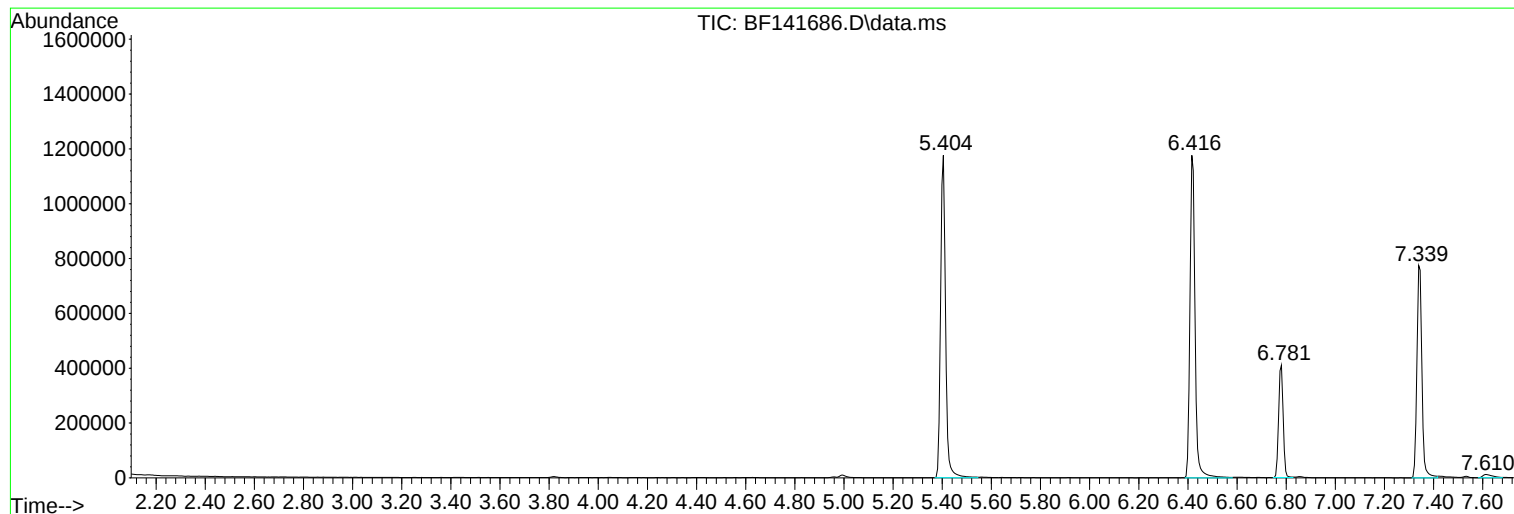

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141686.D
Acq On : 19 Feb 2025 20:39
Operator : RC/JU
Sample : Q1383-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-11-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141686.D
Acq On : 19 Feb 2025 20:39
Operator : RC/JU
Sample : Q1383-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-11-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------