

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
 Data File : BF141687.D
 Acq On : 19 Feb 2025 21:09
 Operator : RC/JU
 Sample : Q1383-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-TC-12-021725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141687.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.404	557	563	587	rBV	1226685	1771318	80.95%	12.555%
2	6.416	730	735	765	rBV	1244123	1819939	83.17%	12.899%
3	6.781	792	797	806	rBV	426819	543663	24.84%	3.853%
4	7.345	887	893	920	rBV	834800	1187846	54.28%	8.419%
5	7.610	934	938	956	rBV2	16272	46225	2.11%	0.328%
6	8.063	1009	1015	1034	rBV	515381	721572	32.98%	5.114%
7	9.133	1192	1197	1216	rVB	1673867	2188233	100.00%	15.510%
8	9.816	1307	1313	1327	rBV	575466	802856	36.69%	5.690%
9	10.527	1429	1434	1441	rBV	109019	143677	6.57%	1.018%
10	10.604	1441	1447	1463	rVV	872668	1208026	55.21%	8.562%
11	11.298	1560	1565	1581	rVB	564642	775568	35.44%	5.497%
12	11.827	1650	1655	1669	rBV3	32747	75440	3.45%	0.535%
13	12.880	1828	1834	1845	rBV	1448654	1853131	84.69%	13.135%
14	13.804	1983	1991	2003	rBV10	10125	50884	2.33%	0.361%
15	13.933	2006	2013	2027	rVB	310718	461915	21.11%	3.274%
16	15.380	2252	2259	2270	rBV	266142	458506	20.95%	3.250%




Sum of corrected areas: 14108799

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141687.D
Acq On : 19 Feb 2025 21:09
Operator : RC/JU
Sample : Q1383-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-12-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

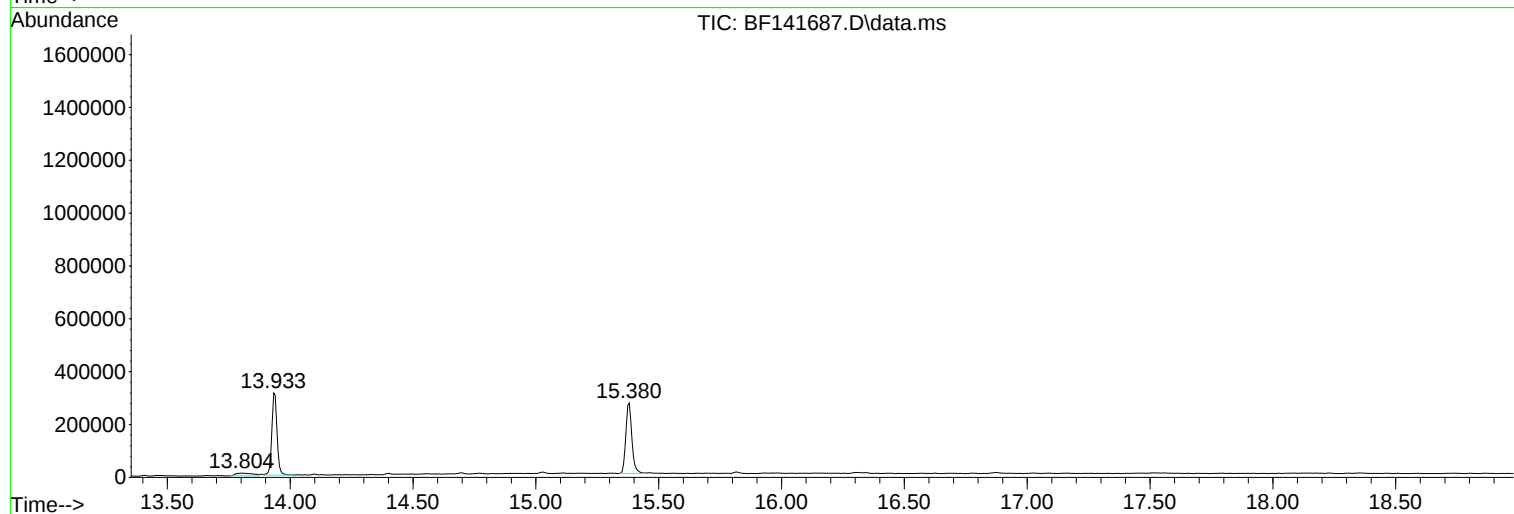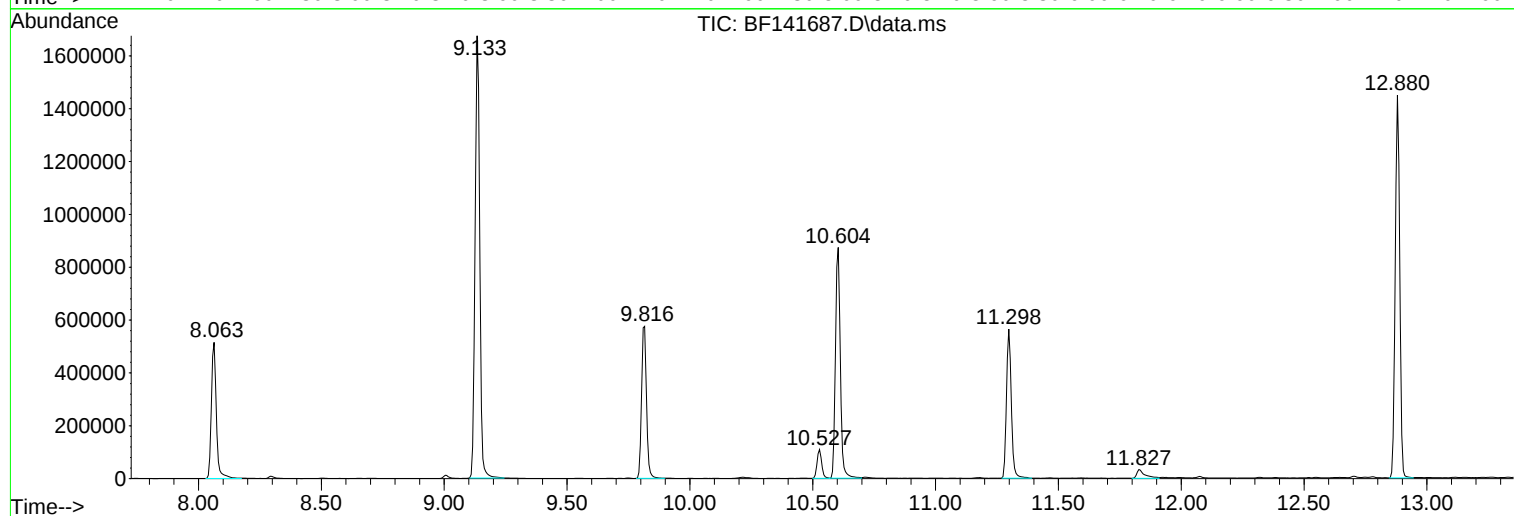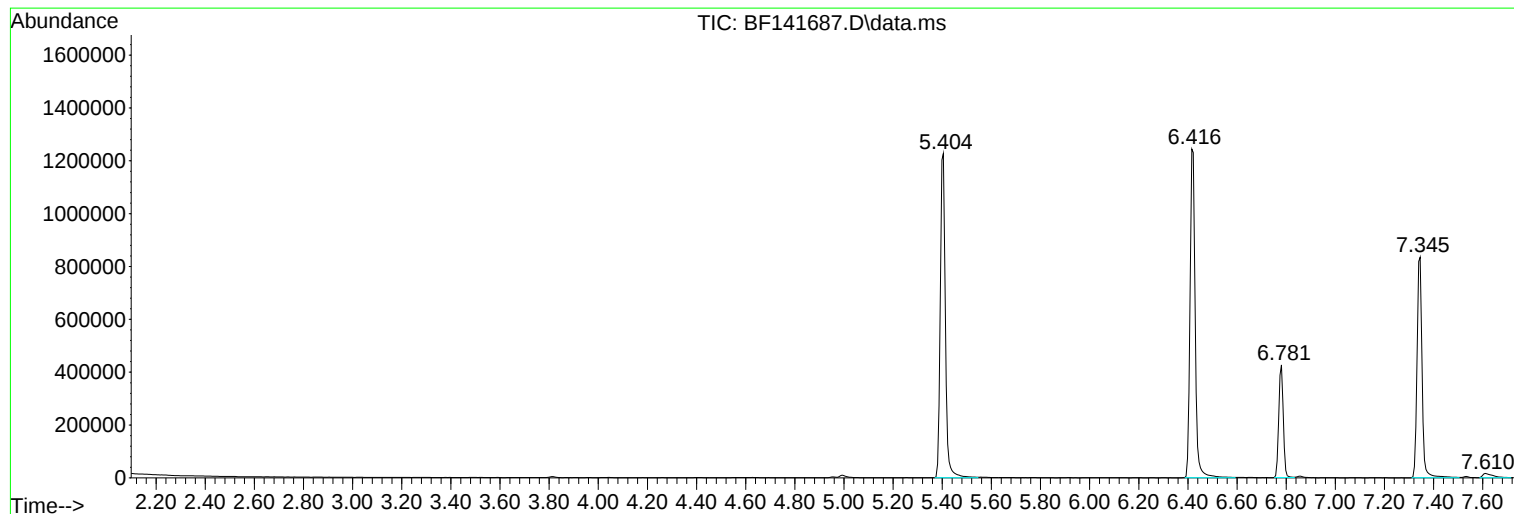

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141687.D
Acq On : 19 Feb 2025 21:09
Operator : RC/JU
Sample : Q1383-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-12-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141687.D
Acq On : 19 Feb 2025 21:09
Operator : RC/JU
Sample : Q1383-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-12-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------