

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
 Data File : BF141688.D
 Acq On : 19 Feb 2025 21:38
 Operator : RC/JU
 Sample : Q1383-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-TC-13-021725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141688.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.404	557	563	591	rBV	1261323	1789577	79.82%	12.517%
2	6.416	730	735	759	rBV	1264671	1838675	82.01%	12.860%
3	6.781	792	797	806	rBV	416616	536188	23.92%	3.750%
4	7.345	887	893	919	rBV	856582	1212215	54.07%	8.479%
5	7.610	933	938	956	rBV	17681	46242	2.06%	0.323%
6	8.063	1009	1015	1035	rBV	507496	719807	32.11%	5.034%
7	9.133	1191	1197	1216	rBV	1688314	2242026	100.00%	15.681%
8	9.810	1307	1312	1327	rBV	570919	796665	35.53%	5.572%
9	10.527	1428	1434	1441	rBV	117407	155870	6.95%	1.090%
10	10.604	1441	1447	1463	rVV	881884	1239150	55.27%	8.667%
11	11.298	1560	1565	1586	rVB	563448	772505	34.46%	5.403%
12	11.827	1650	1655	1673	rBV2	37923	91211	4.07%	0.638%
13	12.880	1828	1834	1844	rBV	1480807	1890724	84.33%	13.224%
14	13.804	1983	1991	2008	rBV	11155	64861	2.89%	0.454%
15	13.933	2008	2013	2022	rVB	312260	444591	19.83%	3.110%
16	15.380	2252	2259	2272	rBV	270114	457197	20.39%	3.198%




Sum of corrected areas: 14297504

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141688.D
Acq On : 19 Feb 2025 21:38
Operator : RC/JU
Sample : Q1383-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-13-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

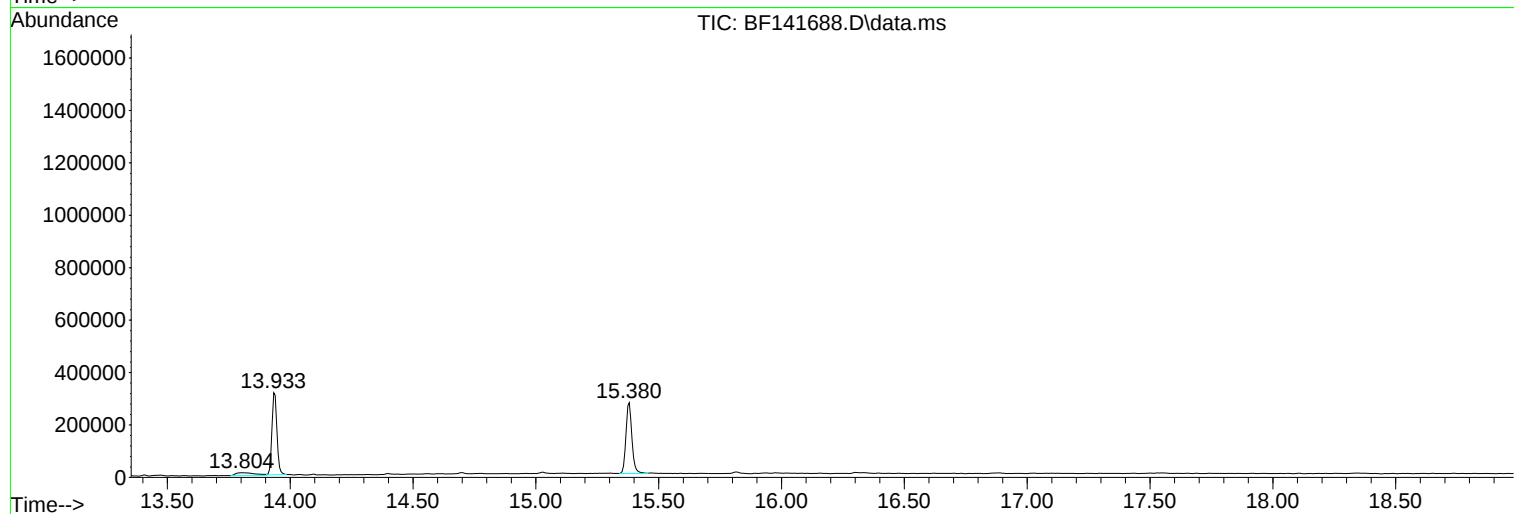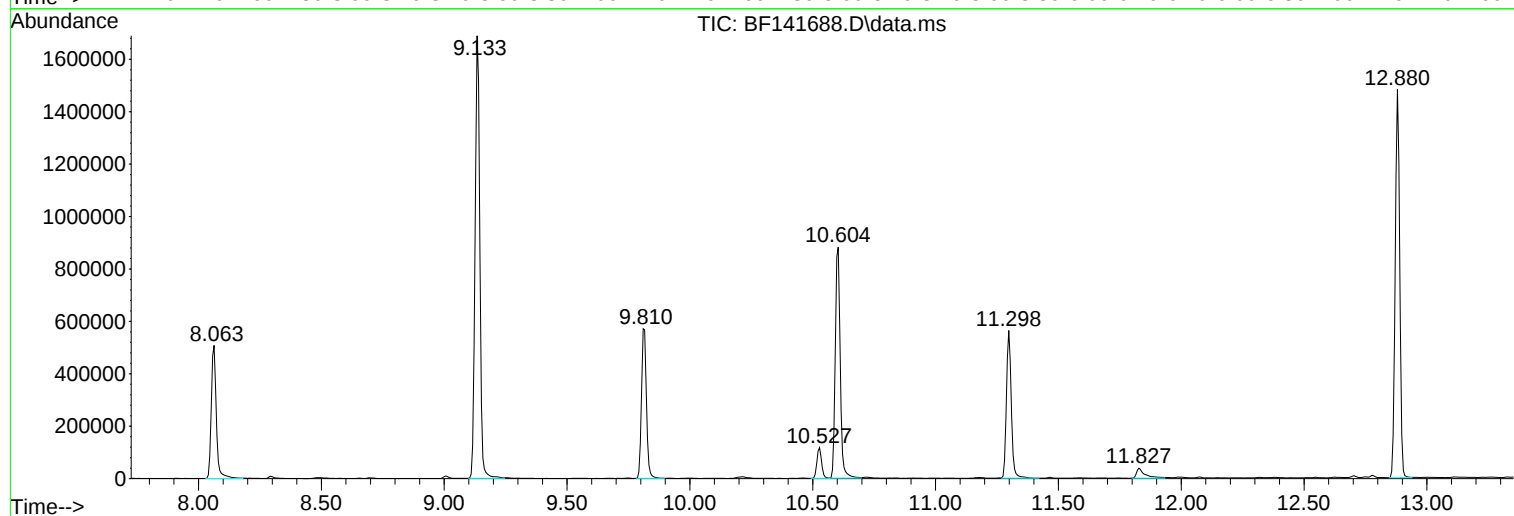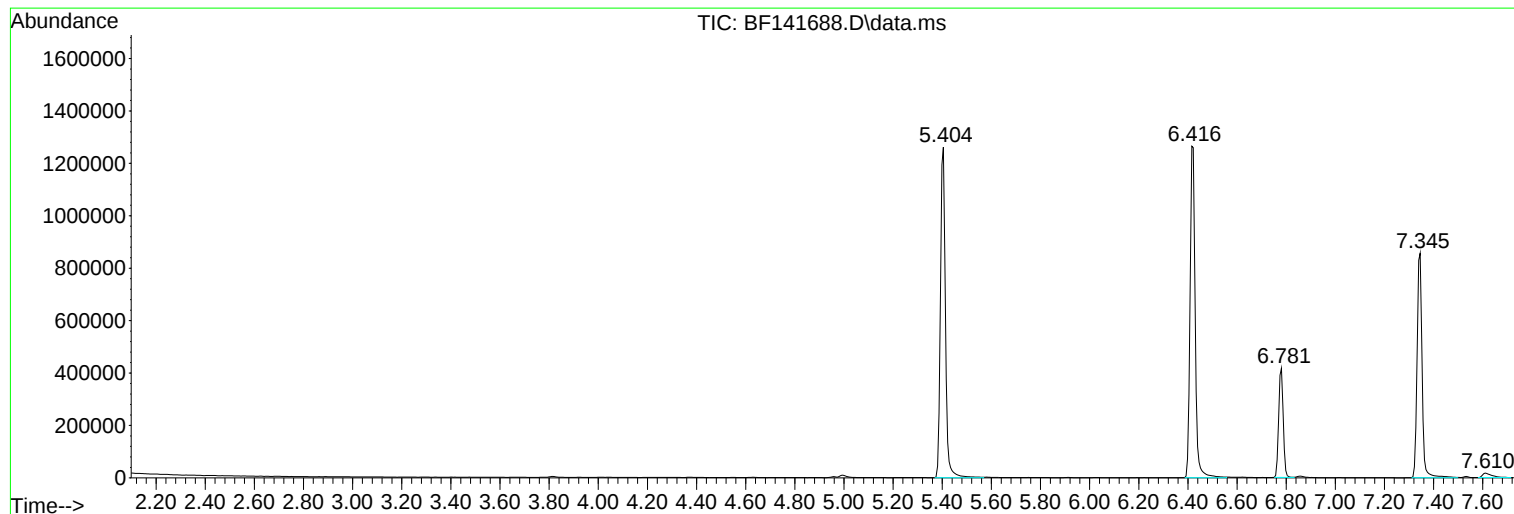

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141688.D
Acq On : 19 Feb 2025 21:38
Operator : RC/JU
Sample : Q1383-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-13-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141688.D
Acq On : 19 Feb 2025 21:38
Operator : RC/JU
Sample : Q1383-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-13-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------