

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
 Data File : BF141689.D
 Acq On : 19 Feb 2025 22:07
 Operator : RC/JU
 Sample : Q1383-07
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-TC-14-021725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141689.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.399	557	562	586	rBV	1322849	1902468	80.78%	12.857%
2	6.422	730	736	763	rBV	1318731	1937117	82.25%	13.091%
3	6.781	791	797	806	rBV	405244	524136	22.26%	3.542%
4	7.345	887	893	921	rBV	891204	1274037	54.10%	8.610%
5	7.610	933	938	951	rBV	15968	41718	1.77%	0.282%
6	8.063	1009	1015	1034	rBV	493561	698454	29.66%	4.720%
7	9.134	1192	1197	1209	rBV	1816477	2355081	100.00%	15.916%
8	9.810	1307	1312	1325	rBV	553015	769408	32.67%	5.200%
9	10.528	1429	1434	1441	rBV	123066	162914	6.92%	1.101%
10	10.604	1441	1447	1463	rVV	939120	1321076	56.09%	8.928%
11	11.298	1560	1565	1585	rVB	549809	753665	32.00%	5.093%
12	11.828	1650	1655	1674	rBV2	49153	115412	4.90%	0.780%
13	12.880	1828	1834	1846	rBV	1568661	2001775	85.00%	13.528%
14	13.798	1983	1990	2008	rBV	13202	73644	3.13%	0.498%
15	13.933	2008	2013	2027	rVB	301062	429312	18.23%	2.901%
16	15.380	2253	2259	2270	rBV	258629	437060	18.56%	2.954%




Sum of corrected areas: 14797277

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141689.D
Acq On : 19 Feb 2025 22:07
Operator : RC/JU
Sample : Q1383-07
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-14-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

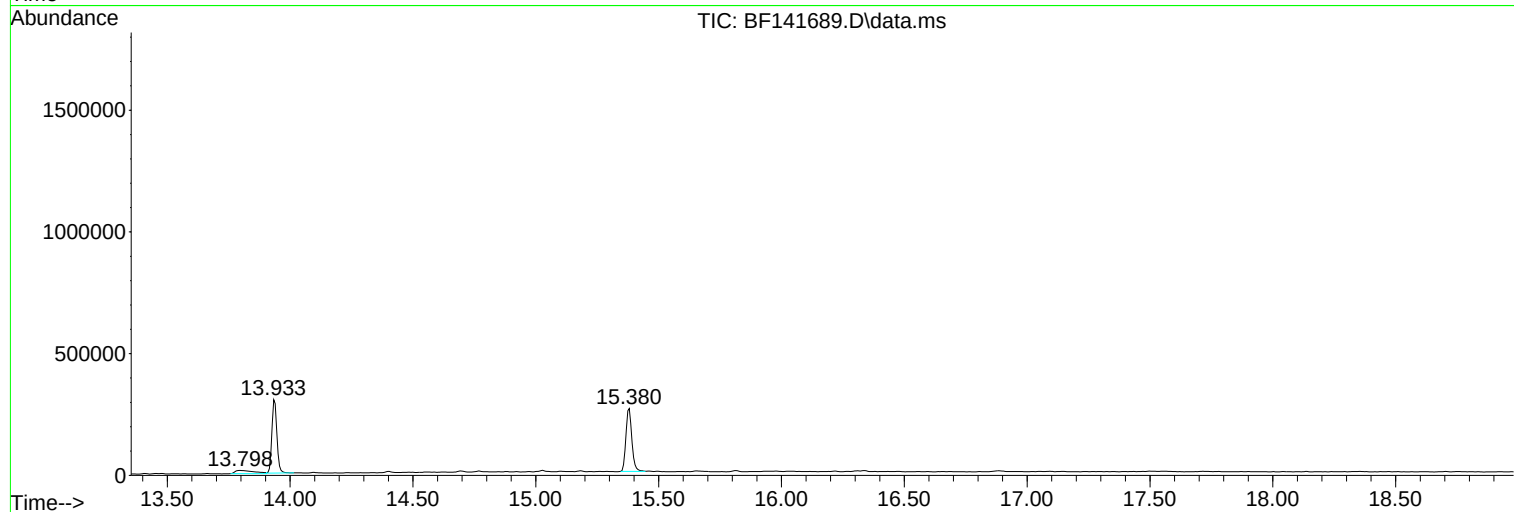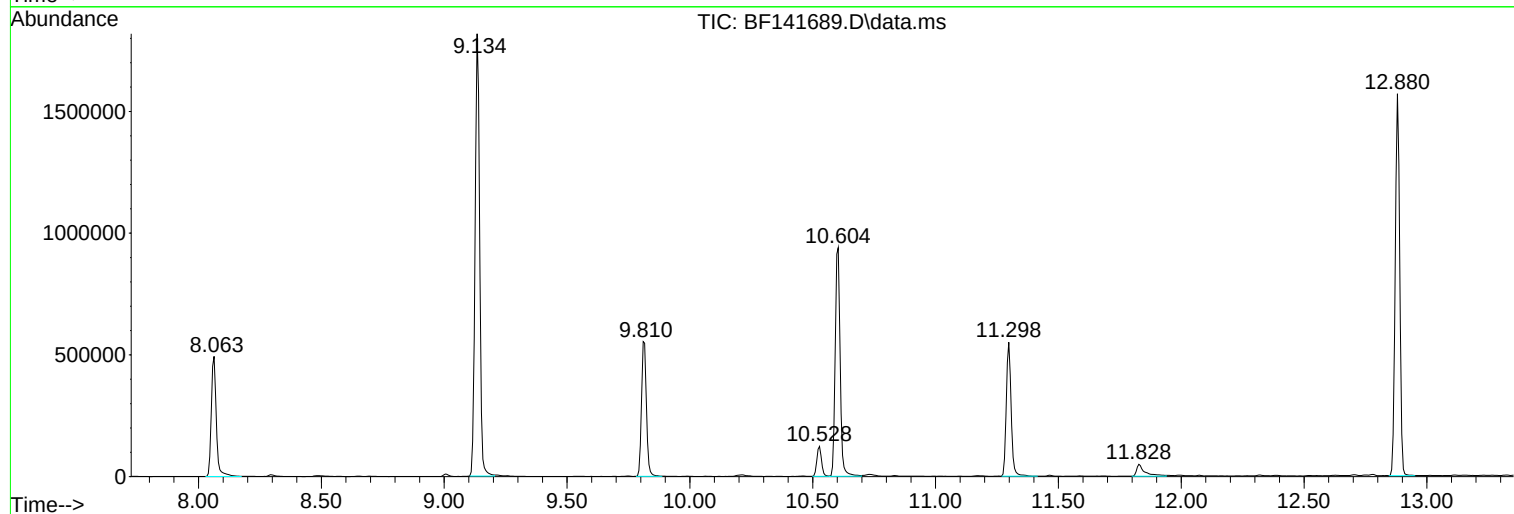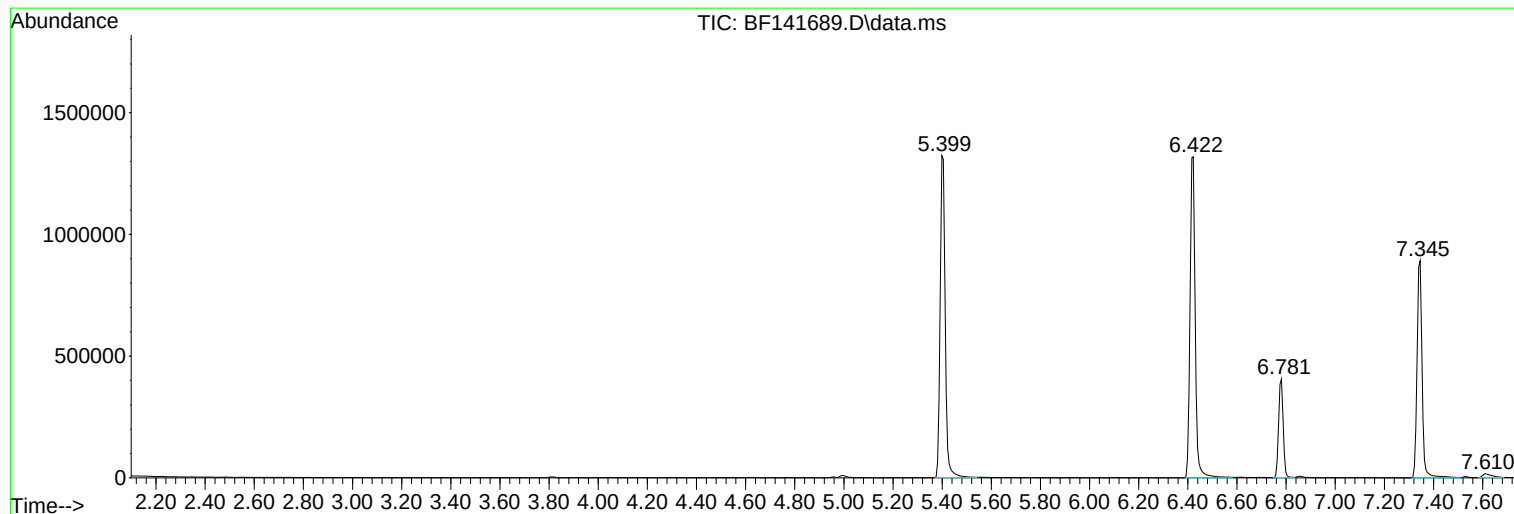

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141689.D
Acq On : 19 Feb 2025 22:07
Operator : RC/JU
Sample : Q1383-07
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-14-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141689.D
Acq On : 19 Feb 2025 22:07
Operator : RC/JU
Sample : Q1383-07
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-14-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------