

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF022015\
 Data File : BF077386.D
 Acq On : 20 Feb 2015 17:17
 Operator : TP/IZ
 Sample : G1302-03RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FYMW-08ARE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.967	6	7	23	rVB3	60532	161529	10.32%	0.967%
2	1.390	42	44	47	rVB2	13506	16934	1.08%	0.101%
3	1.641	62	66	68	rBV	464348	741581	47.38%	4.438%
4	1.812	78	81	84	rVB	573518	746246	47.68%	4.466%
5	1.892	86	88	96	rBV	186779	270368	17.27%	1.618%
6	4.544	315	320	324	rBV	17865	28179	1.80%	0.169%
7	5.127	369	371	375	rVV	61298	78585	5.02%	0.470%
8	5.619	412	414	416	rVB	84803	88689	5.67%	0.531%
9	6.133	456	459	461	rBV	9841	16506	1.05%	0.099%
10	6.887	522	525	527	rBV2	71731	135269	8.64%	0.810%
11	7.036	535	538	540	rVB	180745	172967	11.05%	1.035%
12	7.333	561	564	566	rBV	465019	515588	32.94%	3.086%
13	7.424	569	572	575	rVV	10144	19657	1.26%	0.118%
14	7.516	577	580	582	rVV	846203	790323	50.49%	4.730%
15	7.550	582	583	585	rVV	153261	109263	6.98%	0.654%
16	7.642	589	591	593	rVB	43820	36819	2.35%	0.220%
17	7.733	597	599	604	rVB2	18821	40822	2.61%	0.244%
18	7.836	604	608	610	rBV3	8801	17517	1.12%	0.105%
19	8.019	619	624	627	rBV3	659854	821203	52.46%	4.915%
20	8.282	645	647	651	rBV2	120229	125818	8.04%	0.753%
21	8.510	662	667	669	rBV	54131	73821	4.72%	0.442%
22	8.590	672	674	677	rVB2	54241	70289	4.49%	0.421%
23	8.910	699	702	703	rBV	545676	732478	46.80%	4.384%
24	8.945	703	705	706	rVB2	24807	32950	2.11%	0.197%
25	8.967	706	707	710	rVB2	17526	23654	1.51%	0.142%
26	9.607	761	763	765	rBV	150096	147050	9.39%	0.880%
27	10.248	817	819	822	rBV	1096375	1228654	78.49%	7.354%
28	10.419	832	834	836	rVB	100728	93420	5.97%	0.559%
29	10.750	861	863	866	rBV	155327	179736	11.48%	1.076%
30	11.036	886	888	890	rBV	18941	18667	1.19%	0.112%
31	11.082	890	892	894	rBV	973064	892407	57.01%	5.341%
32	11.231	903	905	906	rBV	25835	31367	2.00%	0.188%
33	11.265	906	908	910	rVV	39984	51995	3.32%	0.311%
34	11.311	910	912	915	rVV	15373	29998	1.92%	0.180%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF022015\
 Data File : BF077386.D
 Acq On : 20 Feb 2015 17:17
 Operator : TP/IZ
 Sample : G1302-03RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FYMW-08ARE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.608	936	938	941	rBV2	62937	72931	4.66%	0.436%
36	11.665	941	943	945	rVB	28700	26722	1.71%	0.160%
37	11.768	950	952	954	rVV	36619	36002	2.30%	0.215%
38	11.836	956	958	964	rVB2	15860	20832	1.33%	0.125%
39	11.985	968	971	973	rBV	471722	482724	30.84%	2.889%
40	12.053	975	977	980	rVB2	104491	134408	8.59%	0.804%
41	12.133	982	984	988	rBV2	11793	22395	1.43%	0.134%
42	12.259	993	995	999	rBV	13067	23941	1.53%	0.143%
43	12.442	1009	1011	1014	rVB	37174	50723	3.24%	0.304%
44	12.511	1014	1017	1019	rBV	209176	261839	16.73%	1.567%
45	12.568	1019	1022	1024	rVV	37653	69675	4.45%	0.417%
46	12.716	1033	1035	1038	rBV2	9015	15788	1.01%	0.094%
47	12.819	1042	1044	1045	rVV	19880	22272	1.42%	0.133%
48	12.876	1045	1049	1051	rVV	66934	66944	4.28%	0.401%
49	12.922	1051	1053	1055	rVV	750506	980156	62.62%	5.866%
50	12.956	1055	1056	1058	rVV	131322	118406	7.56%	0.709%
51	13.048	1062	1064	1066	rVB	20494	20373	1.30%	0.122%
52	13.185	1072	1076	1081	rBV	106500	191371	12.23%	1.145%
53	13.265	1081	1083	1089	rVV2	16629	30678	1.96%	0.184%
54	13.642	1114	1116	1118	rBV	70825	83592	5.34%	0.500%
55	13.928	1138	1141	1143	rBV	29952	27723	1.77%	0.166%
56	14.237	1164	1168	1171	rBV4	6304	18324	1.17%	0.110%
57	14.351	1174	1178	1180	rBV2	11600	18113	1.16%	0.108%
58	14.499	1188	1191	1192	rBV	16174	21836	1.40%	0.131%
59	14.625	1200	1202	1205	rBV2	11278	20764	1.33%	0.124%
60	14.739	1209	1212	1215	rVV	106321	139781	8.93%	0.837%
61	14.819	1217	1219	1220	rVB	14792	18497	1.18%	0.111%
62	14.922	1226	1228	1231	rBV	1472252	1565276	100.00%	9.368%
63	15.231	1252	1255	1257	rBV3	17463	25694	1.64%	0.154%
64	15.642	1289	1291	1292	rBV	15759	18577	1.19%	0.111%
65	15.677	1292	1294	1295	rBV	62373	96737	6.18%	0.579%
66	16.122	1330	1333	1342	rBV	648102	892677	57.03%	5.343%
67	16.248	1342	1344	1347	rVV	944097	1047095	66.90%	6.267%
68	16.294	1347	1348	1351	rVB	13592	19926	1.27%	0.119%
69	16.557	1369	1371	1376	rBV2	22829	36338	2.32%	0.217%
70	16.991	1406	1409	1413	rBV	43762	74021	4.73%	0.443%
71	17.414	1443	1446	1450	rBV2	22641	41130	2.63%	0.246%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF022015\
Data File : BF077386.D
Acq On : 20 Feb 2015 17:17
Operator : TP/IZ
Sample : G1302-03RE
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FYMW-08ARE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	17.494	1451	1453	1457	rVB	13924	19605	1.25%	0.117%
73	17.837	1480	1483	1485	rBV	23664	46637	2.98%	0.279%
74	18.100	1503	1506	1509	rBV	783126	942079	60.19%	5.638%
75	18.260	1517	1520	1524	rBV2	20069	35469	2.27%	0.212%
76	18.728	1558	1561	1562	rBV	24119	42132	2.69%	0.252%
77	18.774	1562	1565	1569	rVB	53556	112552	7.19%	0.674%
78	19.060	1588	1590	1597	rBV6	11751	32762	2.09%	0.196%
79	19.266	1605	1608	1609	rBV2	12227	24469	1.56%	0.146%
80	19.871	1658	1661	1663	rBV4	10657	26240	1.68%	0.157%
81	19.963	1666	1669	1673	rVV5	13086	34008	2.17%	0.204%
82	20.271	1693	1696	1701	rVB5	14034	37823	2.42%	0.226%


Sum of corrected areas: 16708406

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF022015\
Data File : BF077386.D
Acq On : 20 Feb 2015 17:17
Operator : TP/IZ
Sample : G1302-03RE
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FYMW-08ARE

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

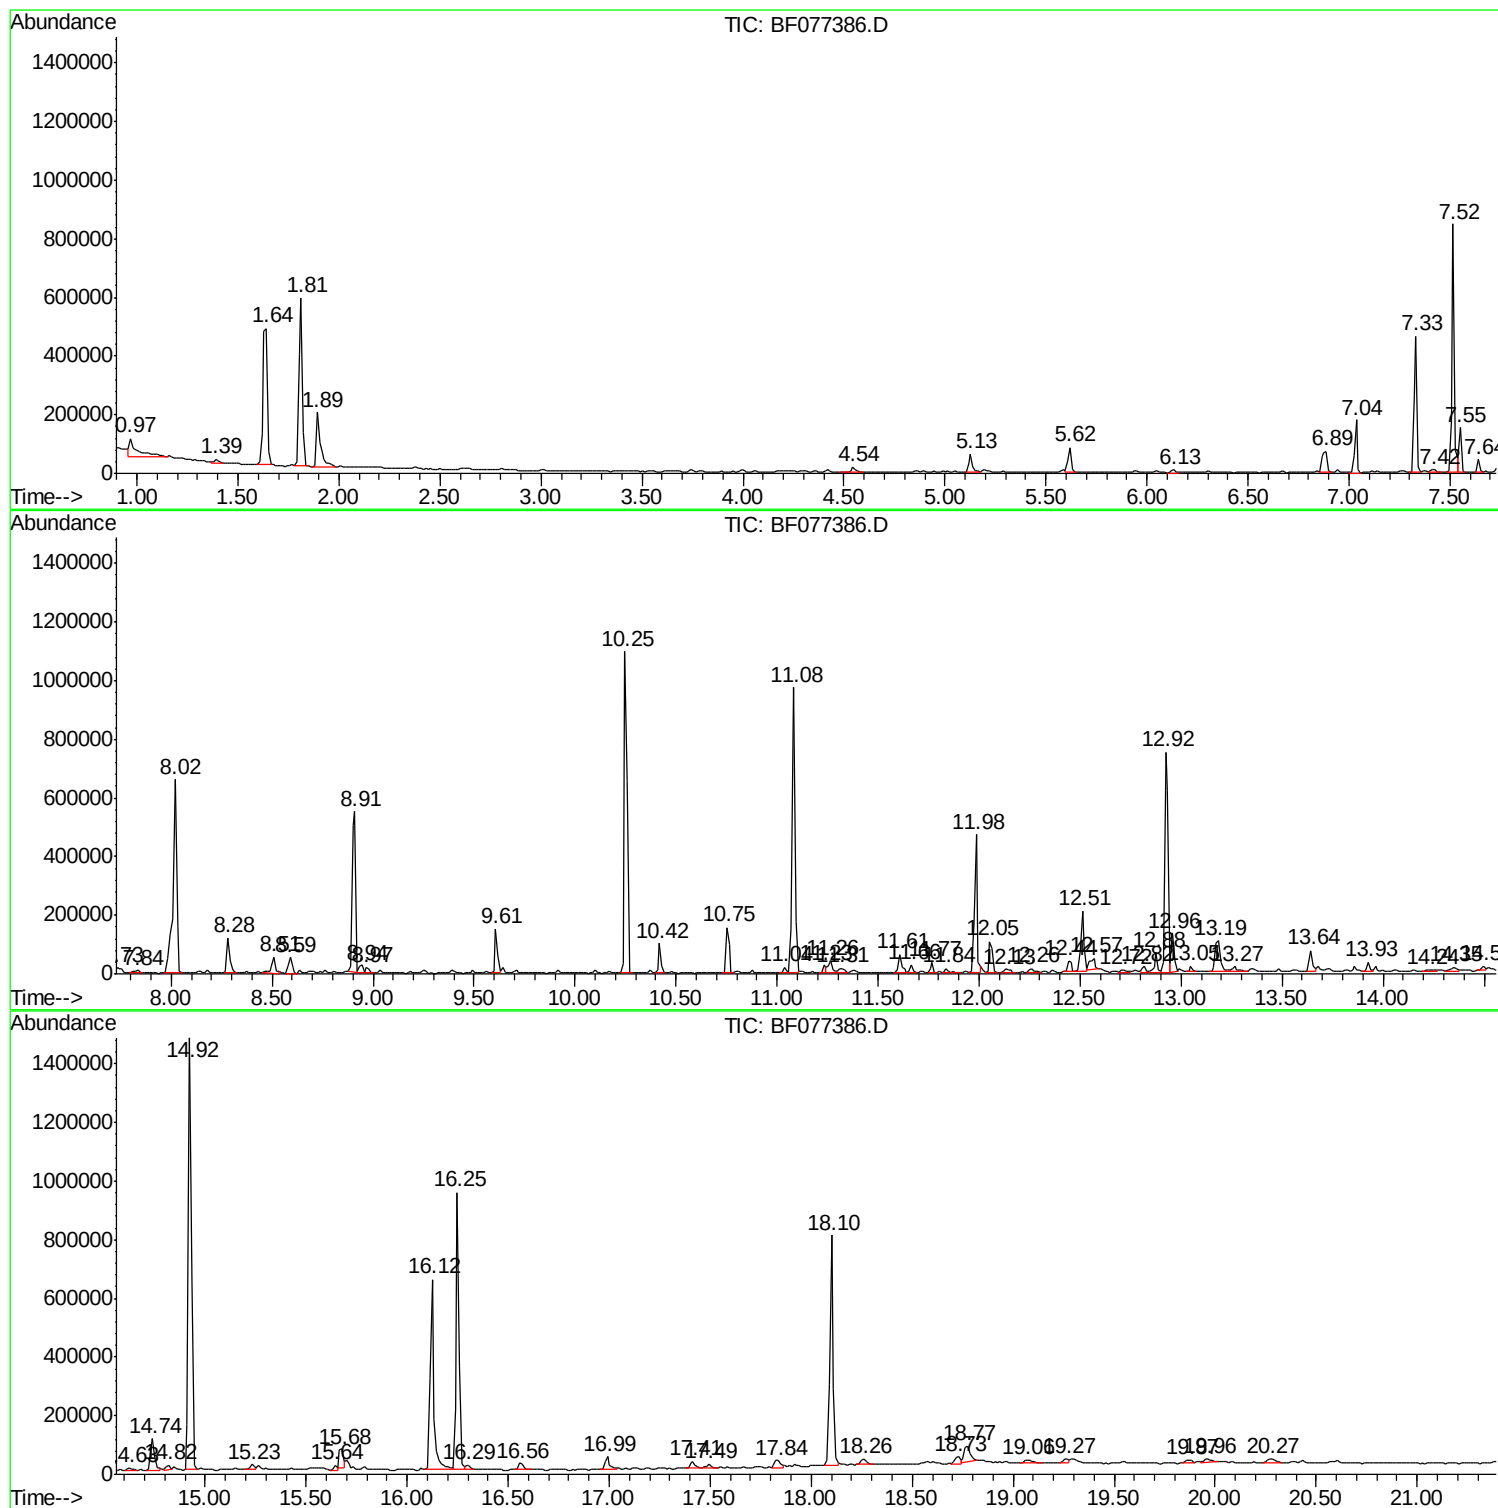

DbaaaPath::ZZ\NRP000M1BNAFNDATA\B0020055\
 DbaaaFile::BB07386DD
 AcqQ00n ::200Febb20055 171717
 Operator::TPPIZ
 Sample::G0300200RE
 Misc::
 ASSVal::99 SampleMultiplier:11

Instrument :
 BNA_F
 ClientSampleId :
 FYMW-08ARE

QcandMebdd::ZZ\NRP000M1BNAFMEH00S8270BB021915MM
 QcandTitle::ASBPBNASSANDABBSF00R55P000NTCALIBRATION

TICLibrary::CC\DATA\BBSSEN055002LL
 TICIntegratIonParameters:LS6CNTPP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
