


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF022015\
 Data File : BF077378.D
 Acq On : 20 Feb 2015 10:23
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 19 16:57:32 2015

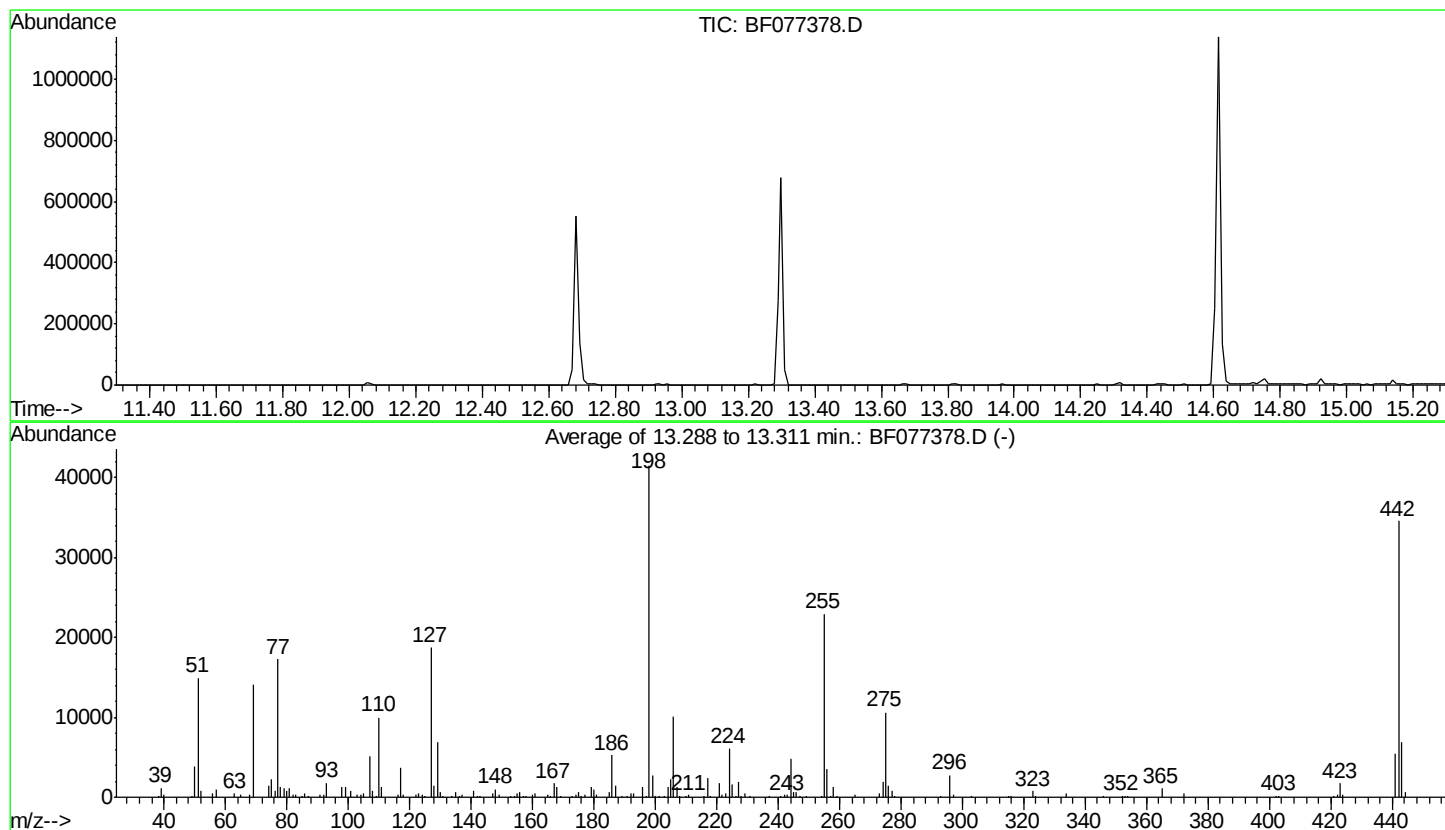

AutoFind: Scans 1085, 1086, 1087; Background Corrected with Scan 1082

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	14955	PASS
68	69	0.00	2	1.9	270	PASS
69	198	0.00	100	33.9	14042	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.0	18680	PASS
197	198	0.00	2	0.5	189	PASS
198	198	100	100	100.0	41468	PASS
199	198	5	9	6.4	2649	PASS
275	198	10	60	25.5	10573	PASS
365	198	1	100	2.6	1091	PASS
441	442	0.01	24	15.6	5385	PASS
442	198	50	100	83.2	34521	PASS
443	442	15	24	20.2	6961	PASS