
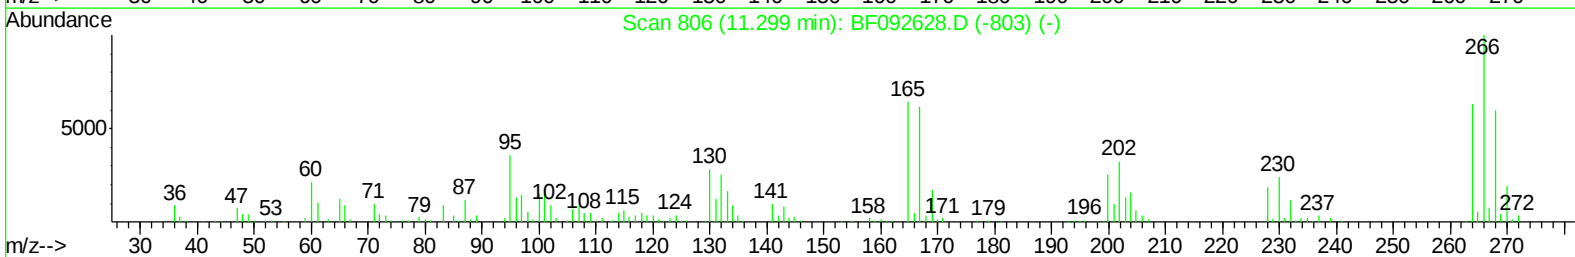
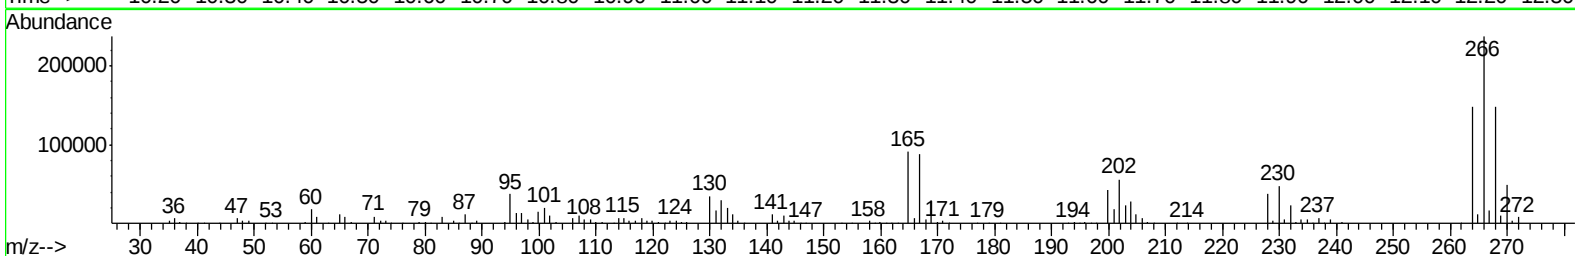


Data File : BF093029.D
Acq On : 20 Feb 2017 15:00
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 05:34:17 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

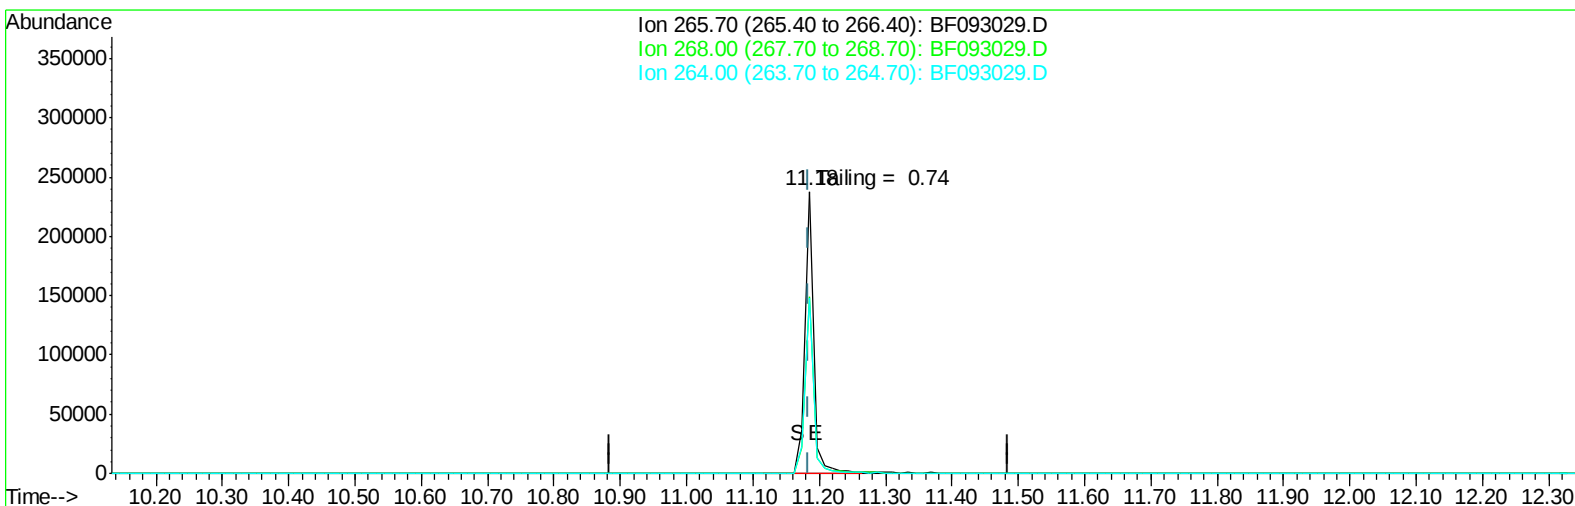

TIC: BF093029.D

(69) Pentachlorophenol (C)




11.185min (-0.000) 0.00ng

response 218262

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	62.63
264.00	62.90	62.15
0.00	0.00	0.00

Data File : BF093029.D
Acq On : 20 Feb 2017 15:00
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 05:34:17 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

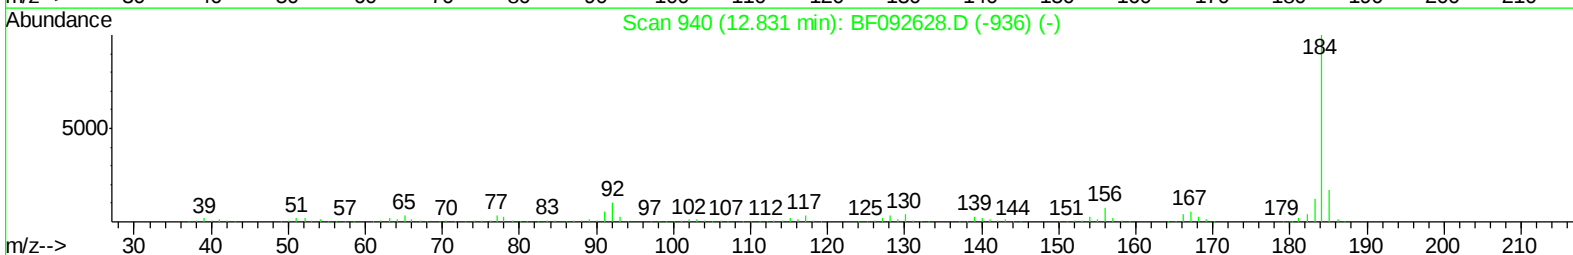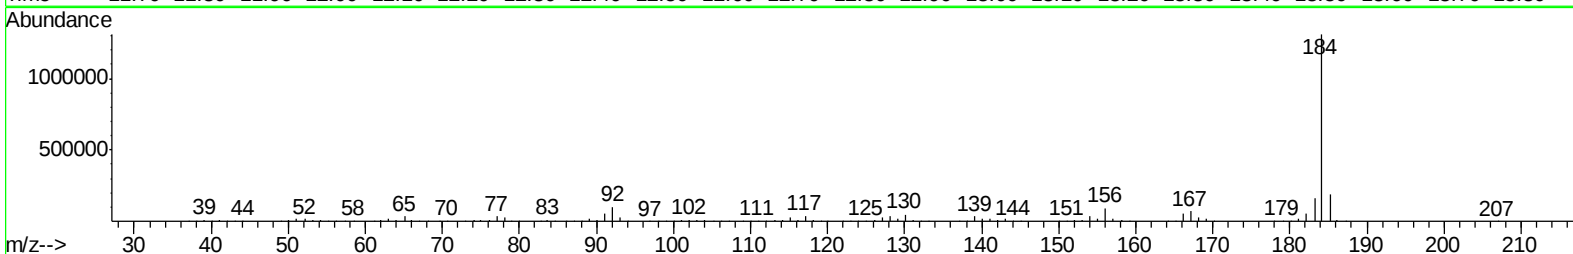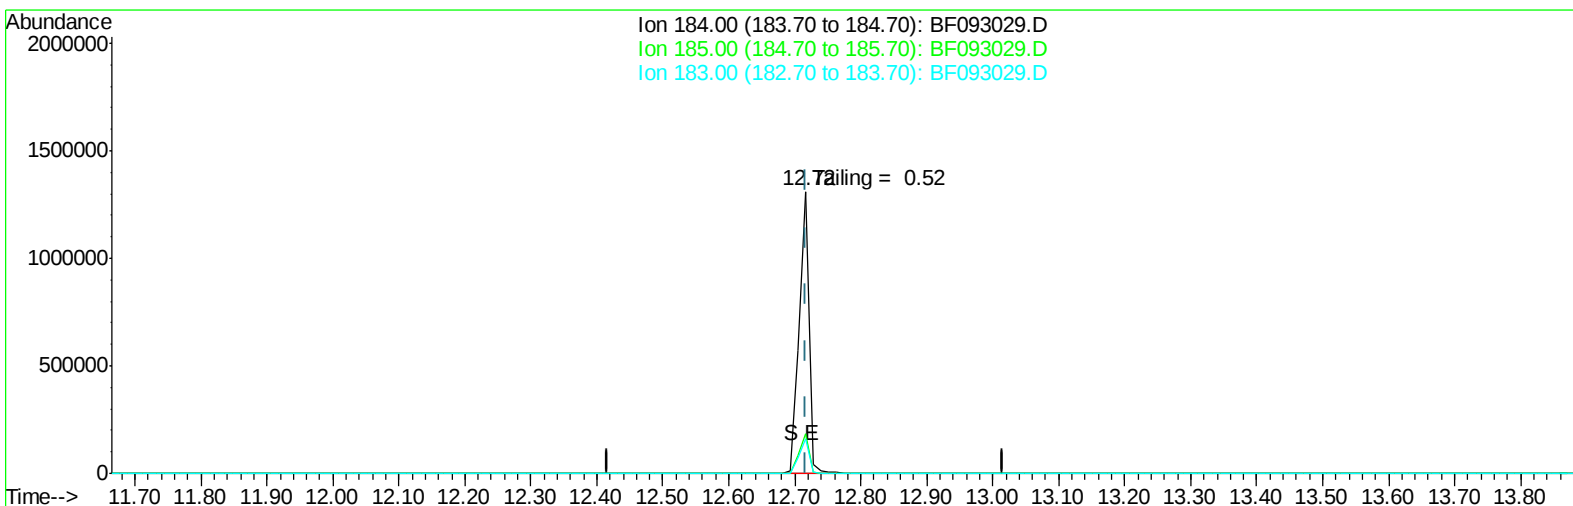

TIC: BF093029.D

(76) Benzidine

12.716min (-0.000) 22829.10ng

response 1356097

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.20
183.00	11.50	12.46
0.00	0.00	0.00