

Data Path : Z:\HPCHEM1\BNA F\DATA\BF022017\
 Data File : BF093042.D
 Acq On : 20 Feb 2017 21:37
 Operator : SJ/MA
 Sample : I1878-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B1-2

Quant Time: Feb 21 00:11:40 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 17 17:31:55 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.84	152	146318	20.00	ng	-0.01
21) Naphthalene-d8	8.13	136	566538	20.00	ng	-0.01
38) Acenaphthene-d10	9.89	164	279191	20.00	ng	0.00
63) Phenanthrene-d10	11.37	188	511312	20.00	ng	-0.01
75) Chrysene-d12	14.01	240	455601	20.00	ng	-0.01
86) Perylene-d12	15.44	264	324926	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.45	112	1032714	121.09	ng	0.00
7) Phenol-d6	6.49	99	1178532	107.40	ng	0.00
23) Nitrobenzene-d5	7.41	82	862934	84.82	ng	-0.01
41) 2,4,6-Tribromophenol	10.68	330	319866	158.41	ng	0.00
44) 2-Fluorobiphenyl	9.22	172	1715746	111.33	ng	0.00
78) Terphenyl-d14	12.96	244	1448571	74.71	ng	-0.01
Target Compounds						
31) Naphthalene	8.16	128	113254	3.94	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF022017\
Data File : BF093042.D
Acq On : 20 Feb 2017 21:37
Operator : SJ/MA
Sample : I1878-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B1-2

Quant Time: Feb 21 00:11:40 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

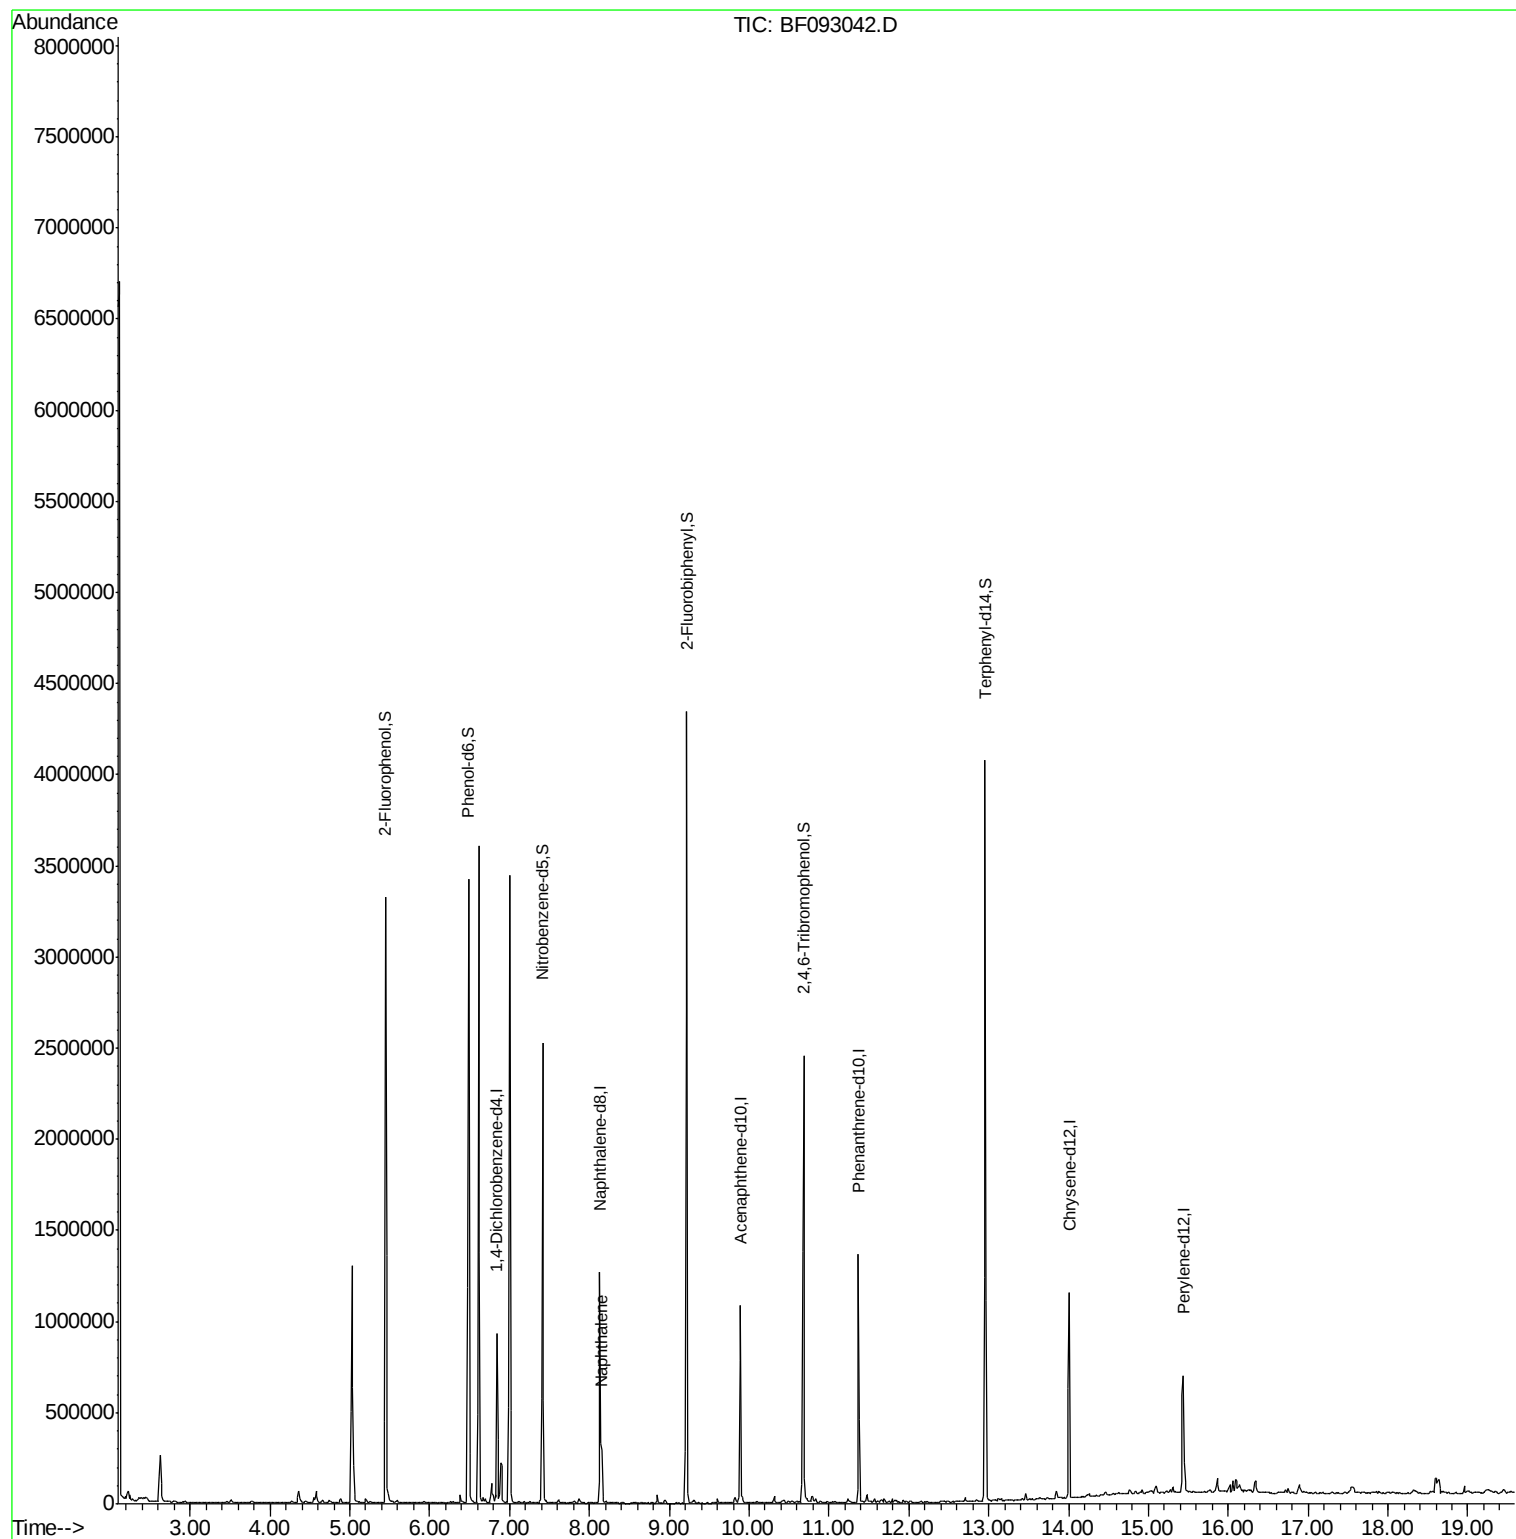

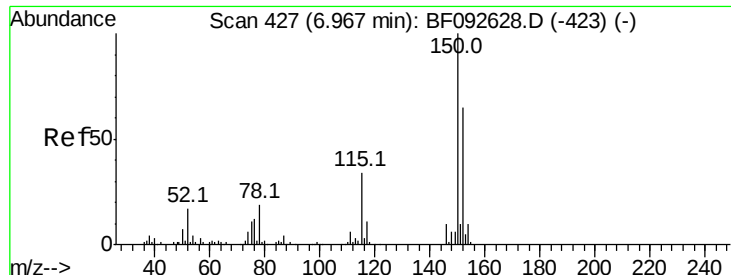

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.84 min Scan# 416

Delta R.T. -0.01 min

Lab File: BF093042.D

Acq: 20 Feb 2017 21:37

Instrument :

BNA_F

ClientSampleId :

B1-2


Tot Ion:152 Resp: 146318

Ion Ratio Lower Upper

152 100

150 162.1 124.9 187.3




115 68.1 46.0 69.0

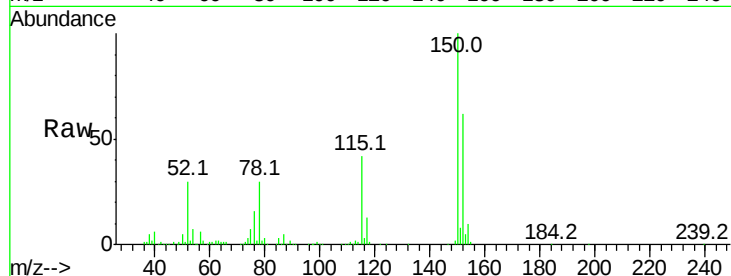

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

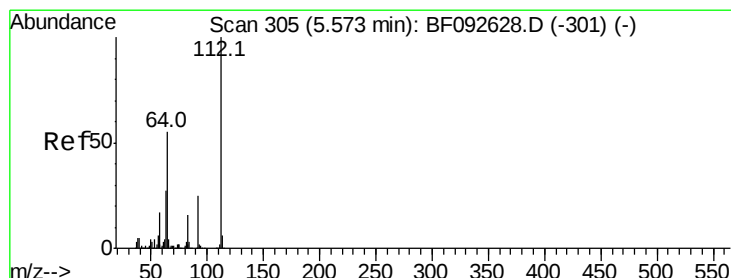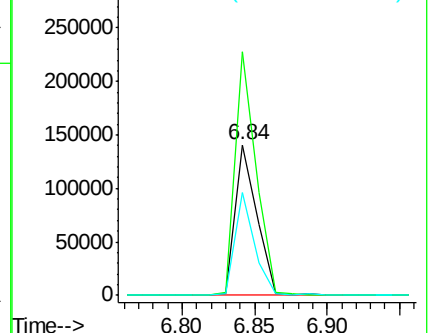

#5

2-Fluorophenol

Concen: 121.09 ng

RT: 5.45 min Scan# 294

Delta R.T. 0.00 min

Lab File: BF093042.D

Acq: 20 Feb 2017 21:37


Tgt Ion:112 Resp: 1032714

Ion Ratio Lower Upper

112 100

64 68.5 46.1 69.1



63 34.3 23.8 35.6

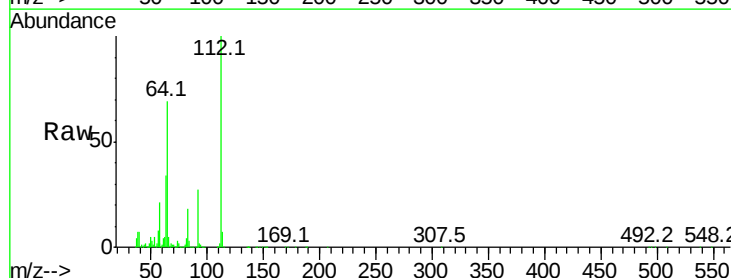


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

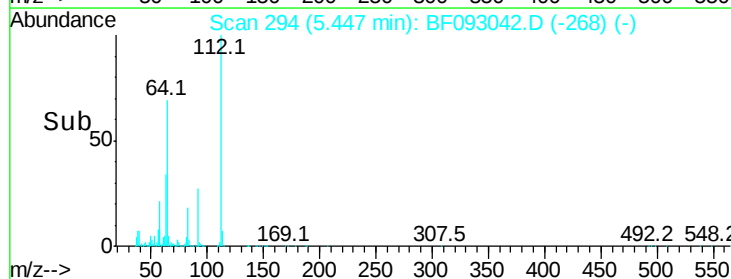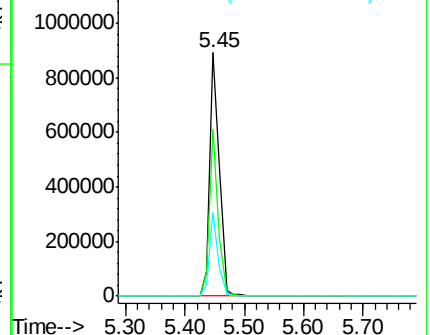

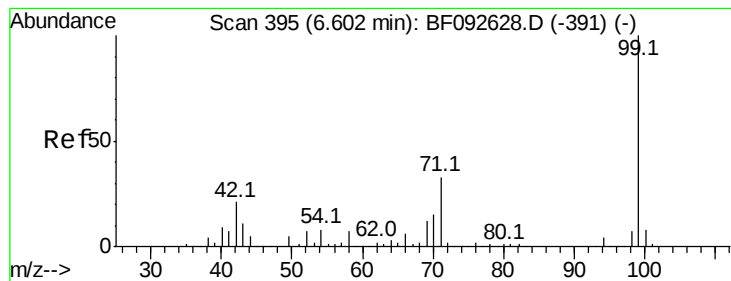

#7

Phenol-d6

Concen: 107.40 ng

RT: 6.49 min Scan# 385

Delta R.T. 0.00 min

Lab File: BF093042.D

Acq: 20 Feb 2017 21:37

Instrument :

BNA_F

ClientSampleId :

B1-2


Tot Ion: 99 Resp: 1178532

Ion Ratio Lower Upper

99 100

42 20.2 15.6 23.4




71 32.7 27.5 41.3

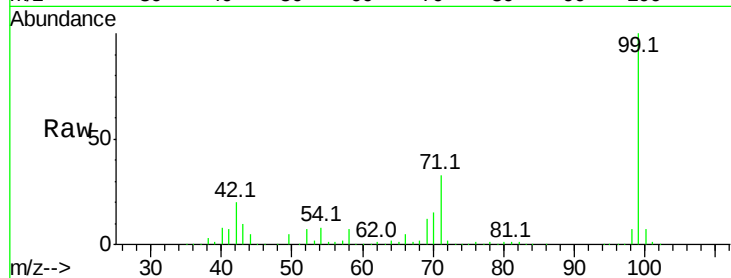

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

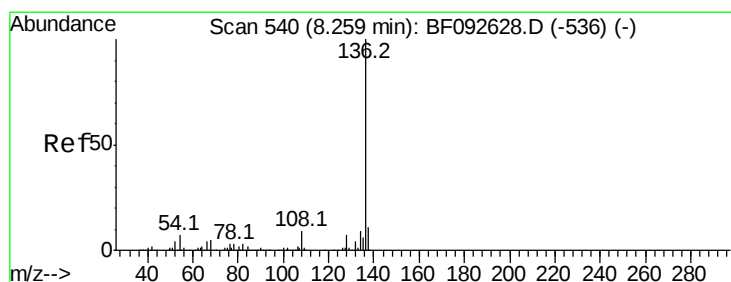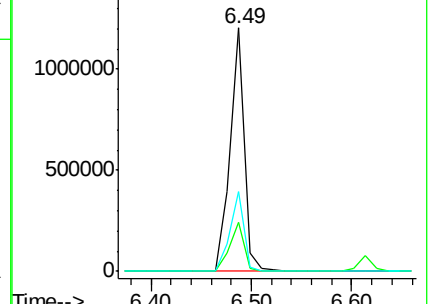

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.13 min Scan# 529

Delta R.T. -0.01 min

Lab File: BF093042.D

Acq: 20 Feb 2017 21:37

Tgt Ion: 136 Resp: 566538


Ion Ratio Lower Upper

136 100

137 11.2 8.4 12.6

54 10.8 4.5 6.7#

68 7.5 3.6 5.4#


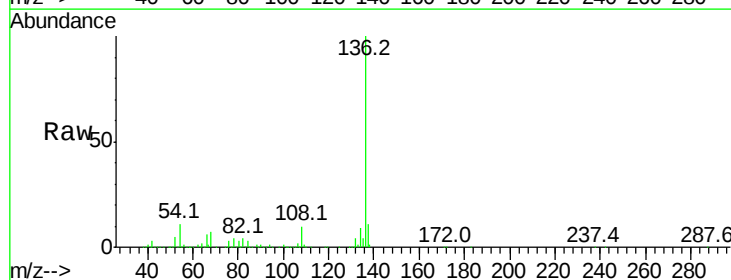



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

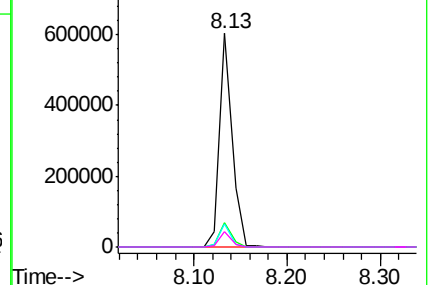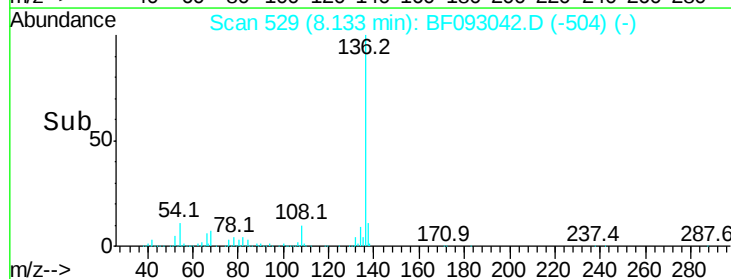







#23
Nitrobenzene-d5
Concen: 84.82 ng
RT: 7.41 min Scan# 466
Delta R.T. -0.01 min
Lab File: BF093042.D
Acq: 20 Feb 2017 21:37

Instrument :
BNA_F
ClientSampleId :
B1-2

Tot Ion: 82 Resp: 862934
Ion Ratio Lower Upper
82 100
128 41.4 34.6 52.0
54 57.5 39.5 59.3

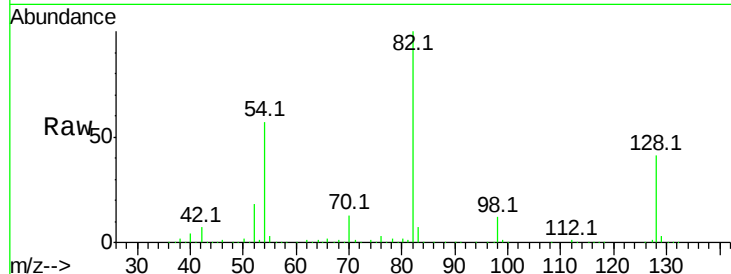


Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

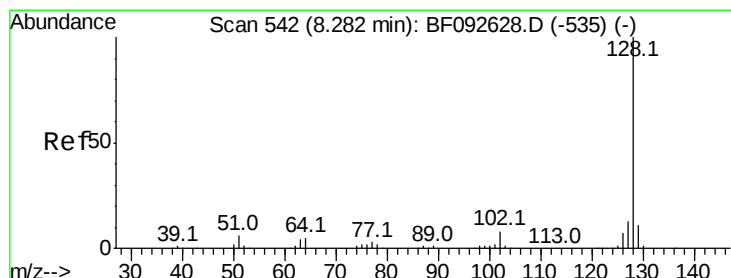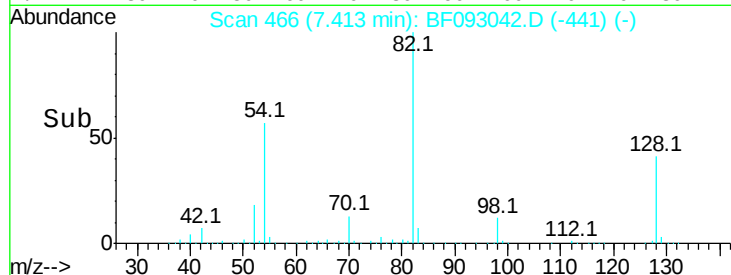
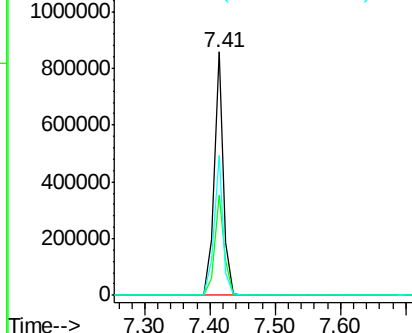



#31
Naphthalene
Concen: 3.94 ng
RT: 8.16 min Scan# 531
Delta R.T. -0.01 min
Lab File: BF093042.D
Acq: 20 Feb 2017 21:37

Tgt Ion: 128 Resp: 113254
Ion Ratio Lower Upper
128 100
129 11.2 9.5 14.3
127 13.2 10.8 16.2

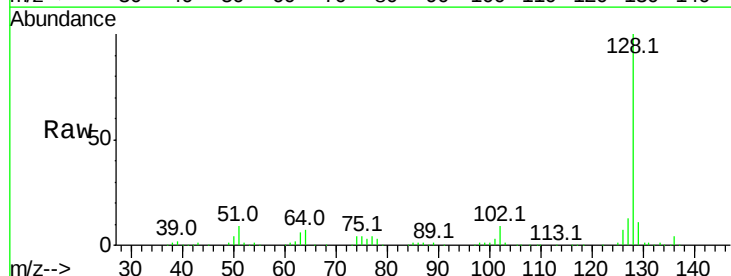

Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E

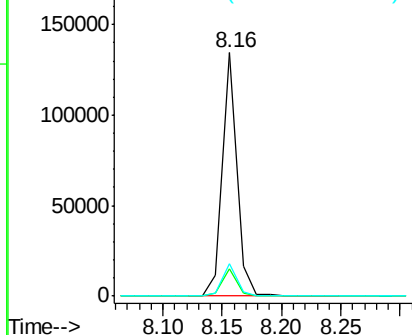


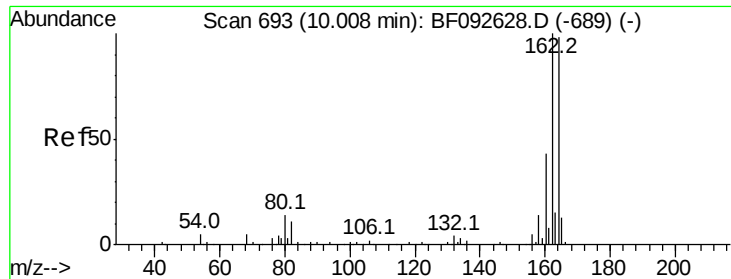



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.89 min Scan# 683
Delta R.T. 0.00 min
Lab File: BF093042.D
Acq: 20 Feb 2017 21:37

Instrument :
BNA_F
ClientSampleId :
B1-2

Tot Ion:164 Resp: 279191
Ion Ratio Lower Upper
164 100
162 107.6 80.2 120.2
160 48.0 36.9 55.3

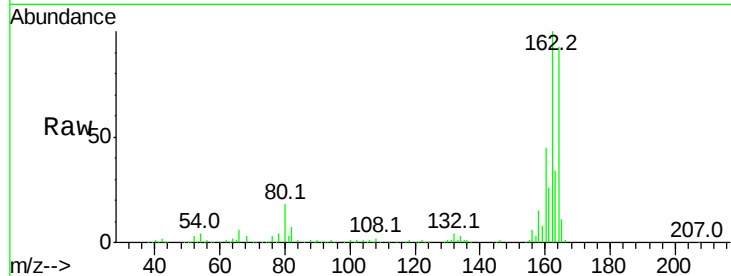


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E


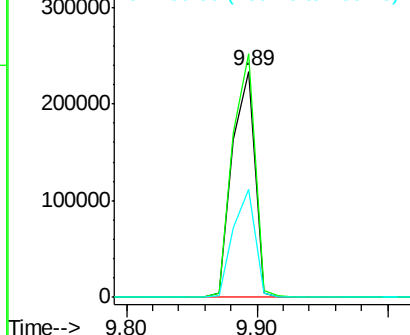



#41
2,4,6-Tribromophenol
Concen: 158.41 ng
RT: 10.68 min Scan# 752
Delta R.T. 0.00 min
Lab File: BF093042.D
Acq: 20 Feb 2017 21:37

Tgt Ion:330 Resp: 319866
Ion Ratio Lower Upper
330 100
332 97.0 77.4 116.2
141 39.7 34.1 51.1

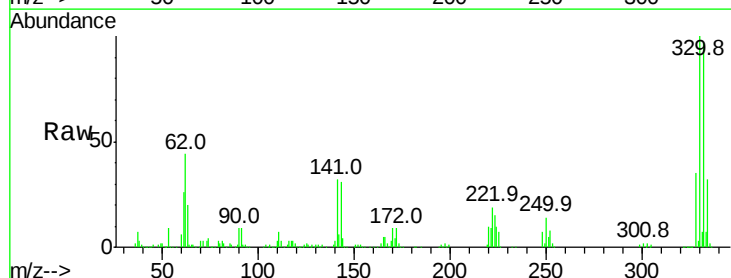

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

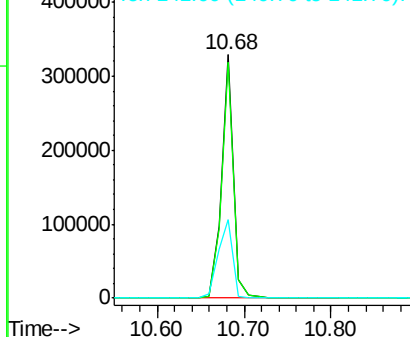




#44
 2-Fluorobiphenyl
 Concen: 111.33 ng
 RT: 9.22 min Scan# 624
 Delta R.T. 0.00 min
 Lab File: BF093042.D
 Acq: 20 Feb 2017 21:37




Instrument :
 BNA_F
 ClientSampleId :
 B1-2

Tot Ion:172 Resp: 1715746

Ion	Ratio	Lower	Upper
172	100		
171	36.8	29.4	44.0
170	24.9	20.2	30.4

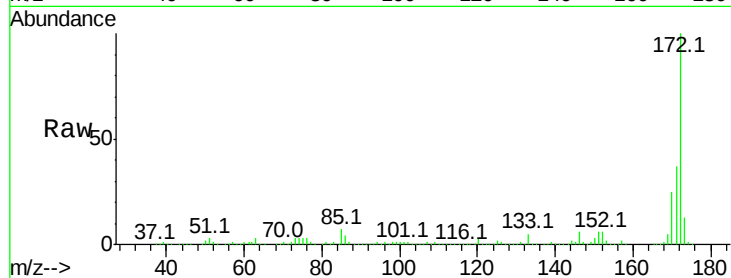


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

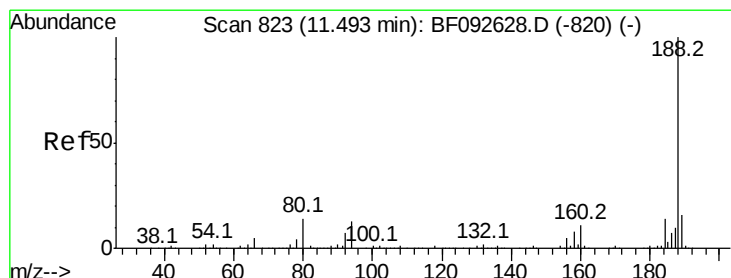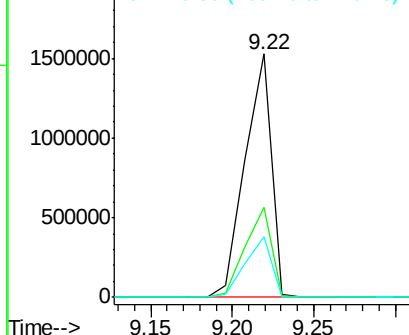



#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.37 min Scan# 812
 Delta R.T. -0.01 min
 Lab File: BF093042.D
 Acq: 20 Feb 2017 21:37


Tgt Ion:188 Resp: 511312

Ion	Ratio	Lower	Upper
188	100		
94	13.5	10.0	15.0
80	14.3	11.2	16.8

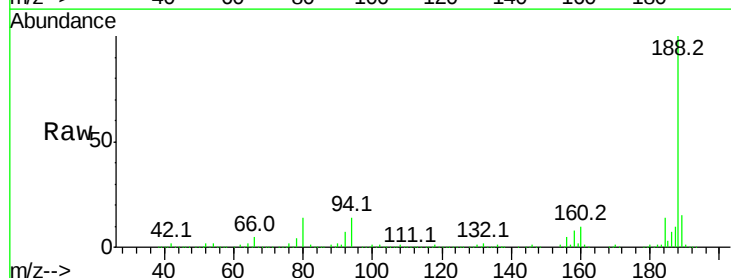

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0

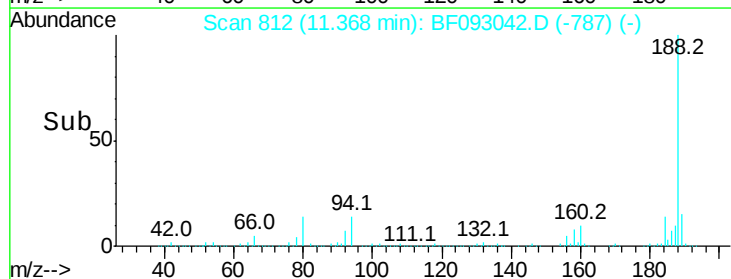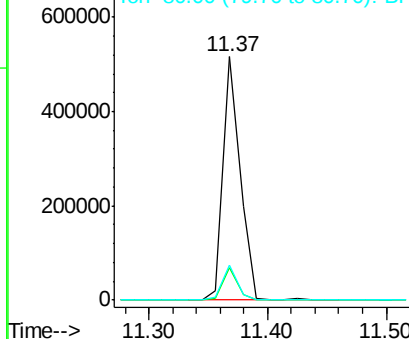



#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.01 min Scan# 1043

Delta R.T. -0.01 min

Lab File: BF093042.D

Acq: 20 Feb 2017 21:37

Instrument :

BNA_F

ClientSampleId :

B1-2


Tot Ion:240 Resp: 455601

Ion Ratio Lower Upper

240 100

120 9.4 12.9 19.3#




236 26.9 20.9 31.3

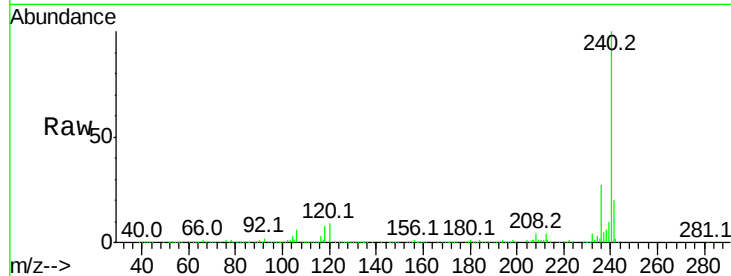

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

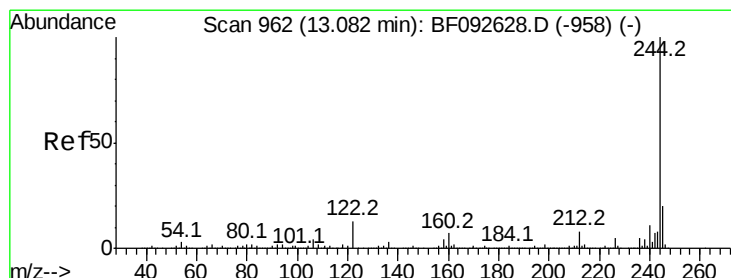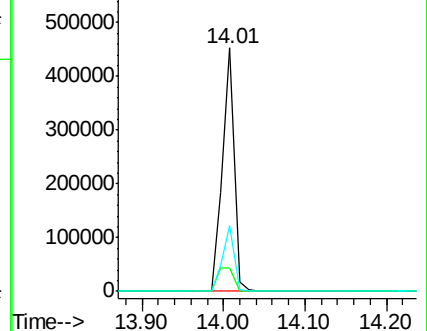

#78

Terphenyl-d14

Concen: 74.71 ng

RT: 12.96 min Scan# 951

Delta R.T. -0.01 min

Lab File: BF093042.D

Acq: 20 Feb 2017 21:37


Tgt Ion:244 Resp: 1448571

Ion Ratio Lower Upper

244 100

212 7.8 6.2 9.2



122 13.8 11.4 17.2

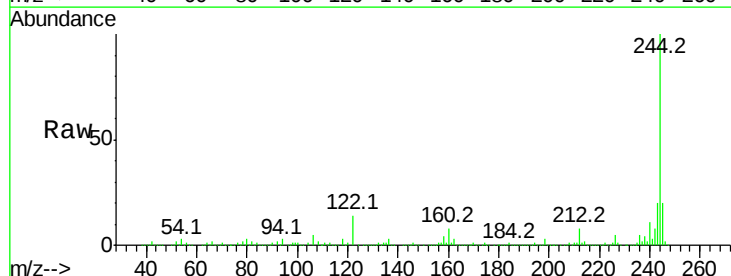


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

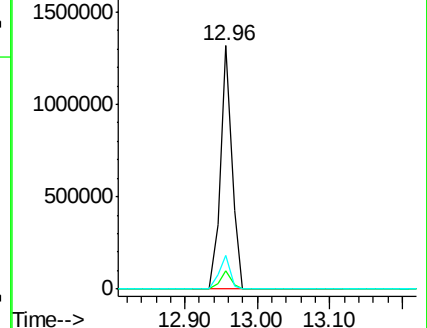


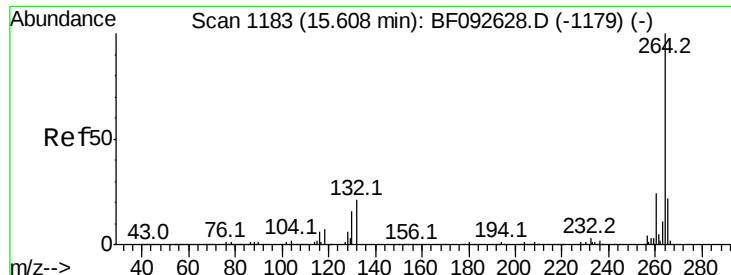

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 15.44 min Scan# 1168
 Delta R.T. -0.01 min
 Lab File: BF093042.D
 Acq: 20 Feb 2017 21:37

Instrument :
 BNA_F
 ClientSampleId :
 B1-2

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.2	19.2	28.8
265	20.8	17.4	26.0

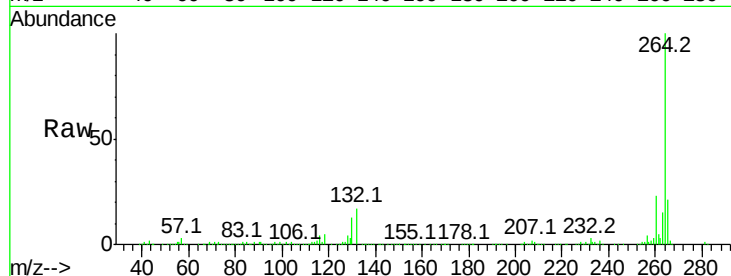

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

