

Data Path : Z:\HPCHEM1\BNA F\DATA\BF022017\
 Data File : BF093064.D
 Acq On : 21 Feb 2017 9:30
 Operator : SJ/MA
 Sample : I1897-02
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 021417-PRRT-F-D-S

Quant Time: Feb 21 13:25:31 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 17 17:31:55 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.84	152	158743	20.00	ng	-0.01
21) Naphthalene-d8	8.13	136	606489	20.00	ng	-0.01
38) Acenaphthene-d10	9.89	164	274771	20.00	ng	0.00
63) Phenanthrene-d10	11.37	188	476248	20.00	ng	-0.01
75) Chrysene-d12	14.01	240	324587	20.00	ng	-0.01
86) Perylene-d12	15.44	264	295185	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.44	112	413967	44.74	ng	-0.01
7) Phenol-d6	6.48	99	330739	27.78	ng	-0.01
23) Nitrobenzene-d5	7.41	82	950190	87.25	ng	-0.01
41) 2,4,6-Tribromophenol	10.68	330	222242	111.83	ng	0.00
44) 2-Fluorobiphenyl	9.22	172	1804948	119.01	ng	0.00
78) Terphenyl-d14	12.96	244	1189029	86.07	ng	-0.01
Target Compounds						Qvalue
49) Dimethylphthalate	9.61	163	81382	4.40	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF022017\
Data File : BF093064.D
Acq On : 21 Feb 2017 9:30
Operator : SJ/MA
Sample : I1897-02
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
021417-PRRT-F-D-S

Quant Time: Feb 21 13:25:31 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

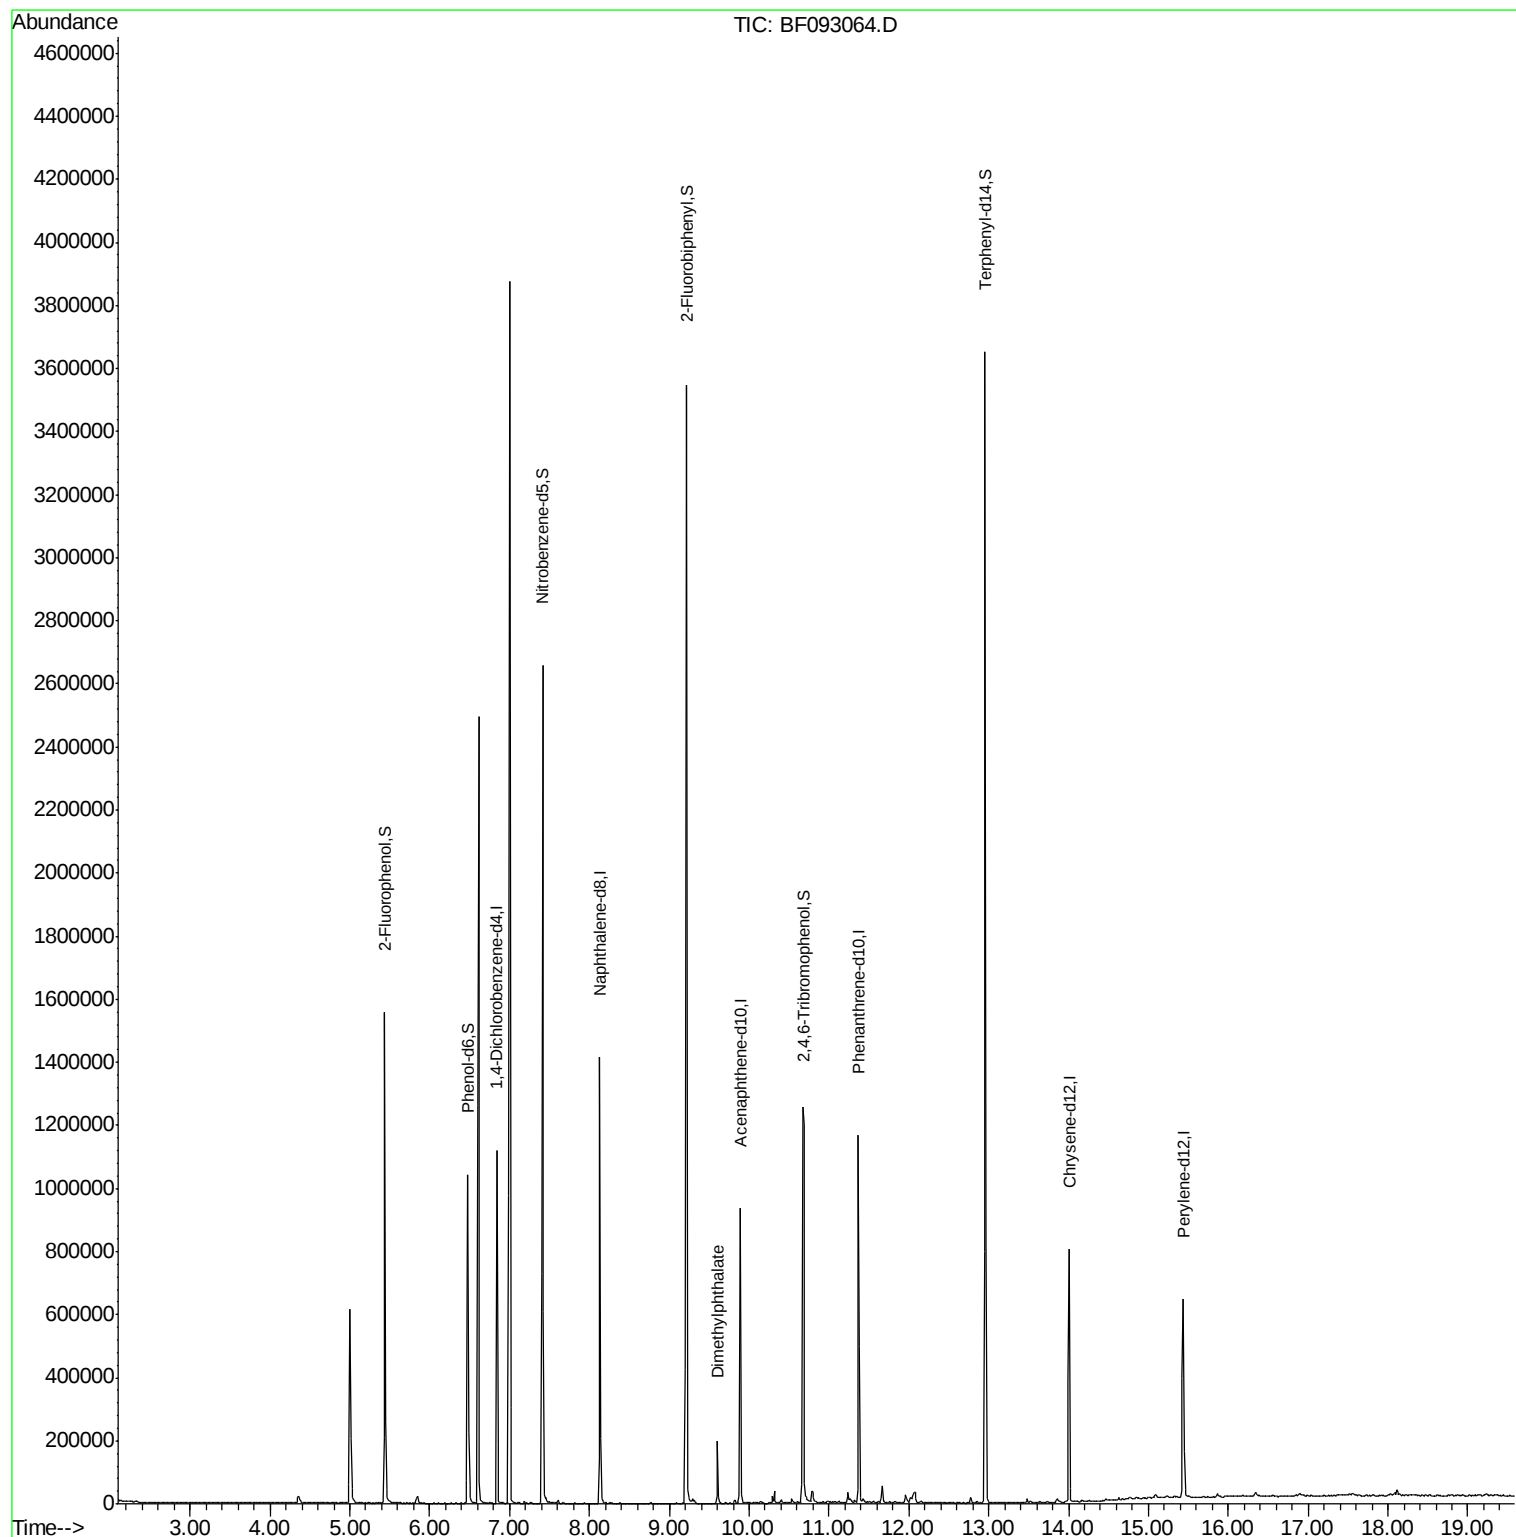

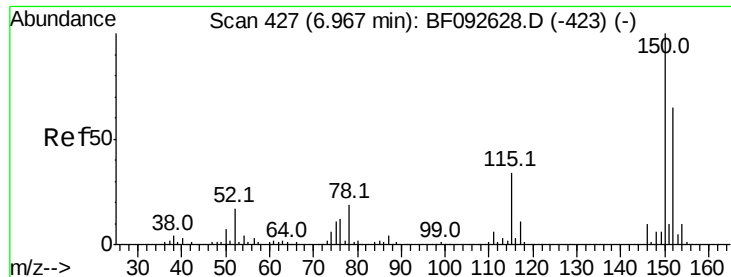

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.84 min Scan# 416

Delta R.T. -0.01 min

Lab File: BF093064.D

Acq: 21 Feb 2017 9:30

Instrument :

BNA_F

ClientSampleId :

021417-PRRT-F-D-S


Tot Ion:152 Resp: 158743

Ion Ratio Lower Upper

152 100

150 157.0 124.9 187.3




115 62.2 46.0 69.0

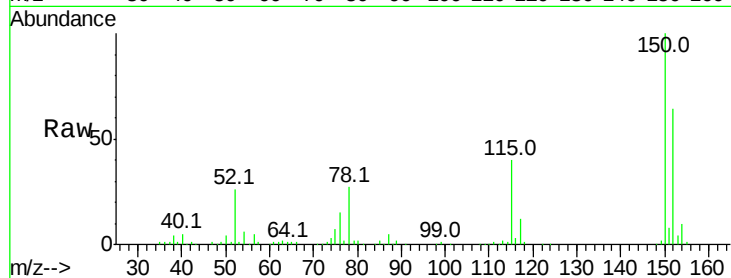

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

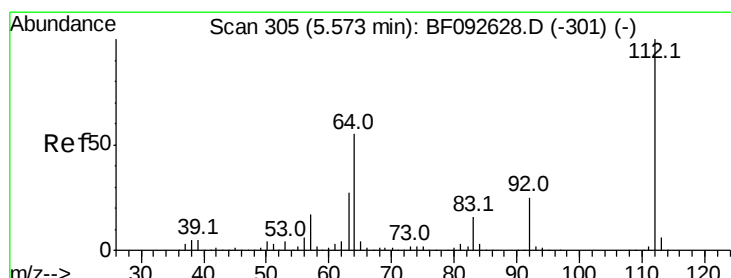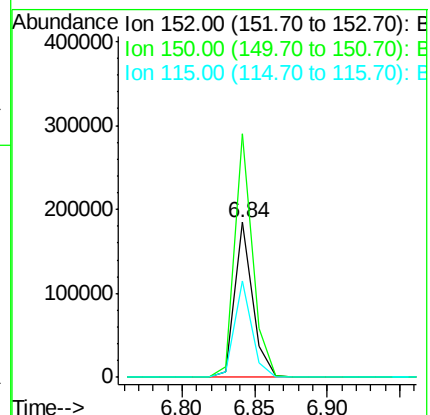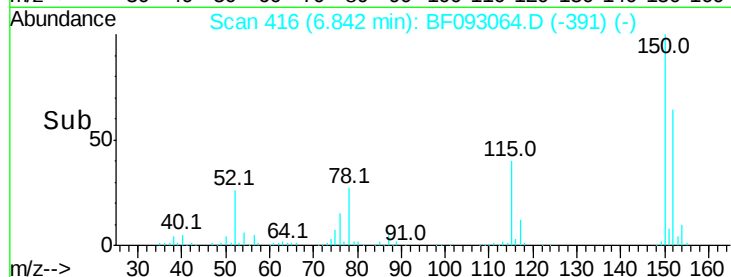

#5

2-Fluorophenol

Concen: 44.74 ng

RT: 5.44 min Scan# 293

Delta R.T. -0.01 min

Lab File: BF093064.D

Acq: 21 Feb 2017 9:30


Tgt Ion:112 Resp: 413967

Ion Ratio Lower Upper

112 100

64 63.6 46.1 69.1



63 31.5 23.8 35.6

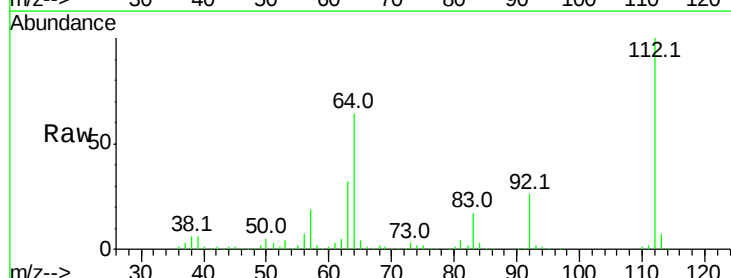


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

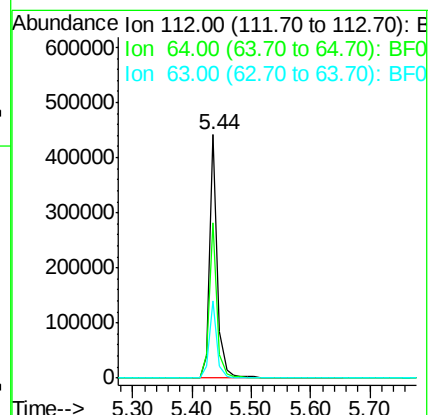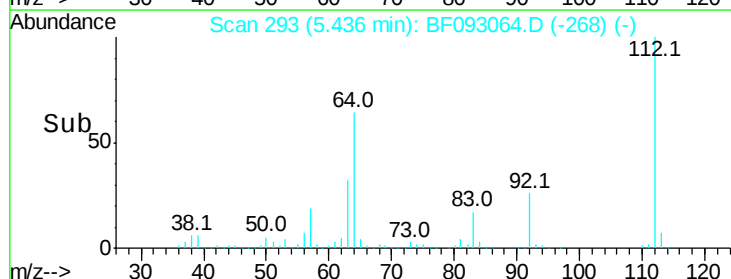

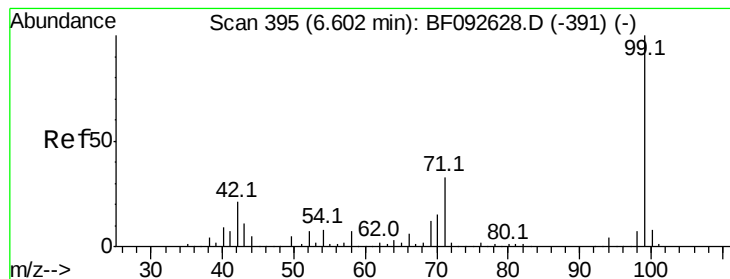

#7

Phenol-d6

Concen: 27.78 ng

RT: 6.48 min Scan# 384

Delta R.T. -0.01 min

Lab File: BF093064.D

Acq: 21 Feb 2017 9:30

Instrument :

BNA_F

ClientSampleId :

021417-PRRT-F-D-S


Tot Ion: 99 Resp: 330739

Ion Ratio Lower Upper

99 100

42 19.0 15.6 23.4




71 31.0 27.5 41.3

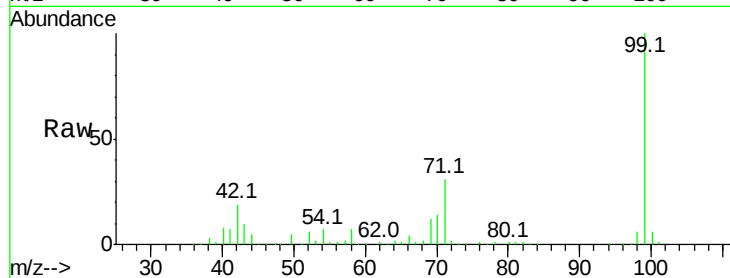

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

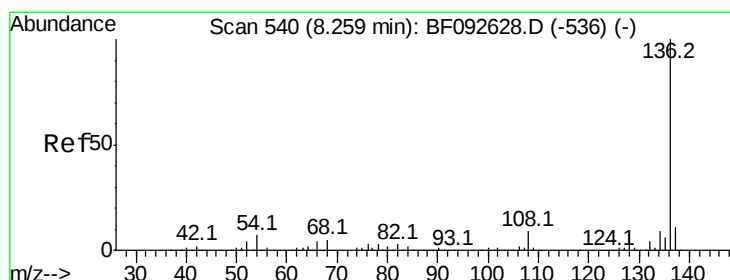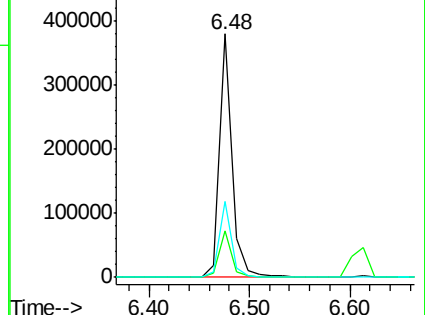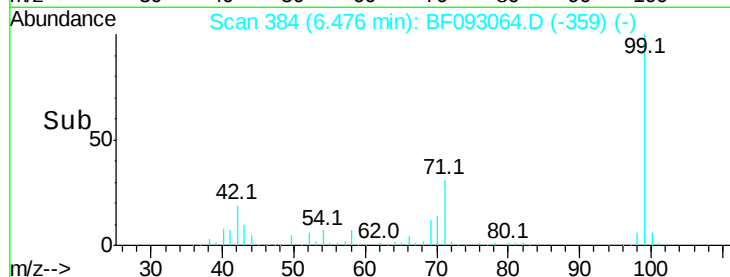

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.13 min Scan# 529

Delta R.T. -0.01 min

Lab File: BF093064.D

Acq: 21 Feb 2017 9:30

Tgt Ion: 136 Resp: 606489


Ion Ratio Lower Upper

136 100

137 10.9 8.4 12.6

54 10.2 4.5 6.7#

68 7.4 3.6 5.4#


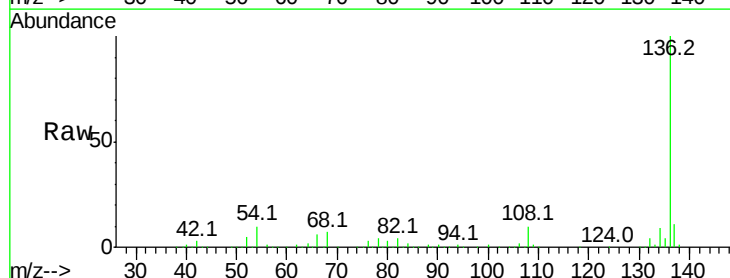


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

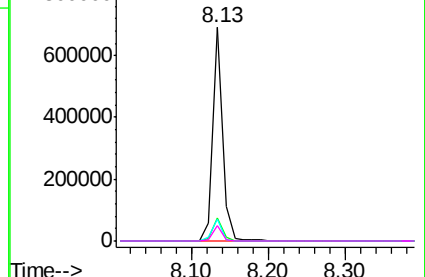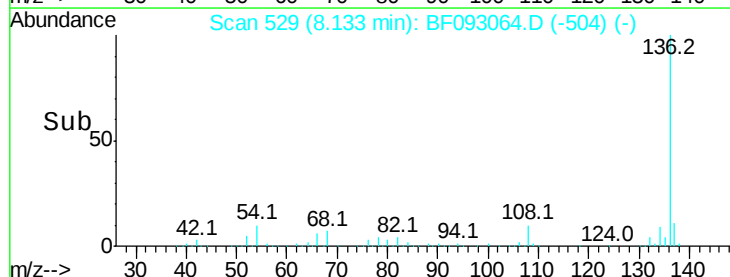







#23
 Nitrobenzene-d5
 Concen: 87.25 ng
 RT: 7.41 min Scan# 466
 Delta R.T. -0.01 min
 Lab File: BF093064.D
 Acq: 21 Feb 2017 9:30

Instrument :
 BNA_F
 ClientSampleId :
 021417-PRRT-F-D-S

Tot Ion	82	Resp	950190
Ion Ratio	Lower	Upper	
82	100		
128	40.9	34.6	52.0
54	57.9	39.5	59.3

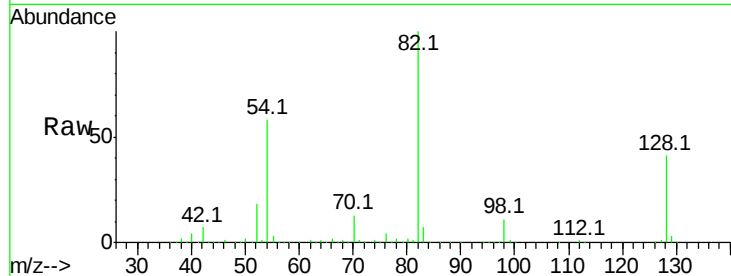


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): BF0
 Ion 54.00 (53.70 to 54.70): BF0

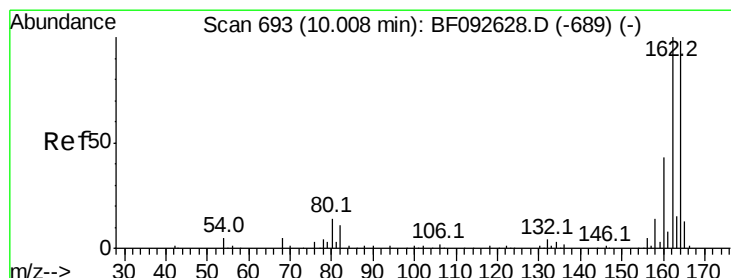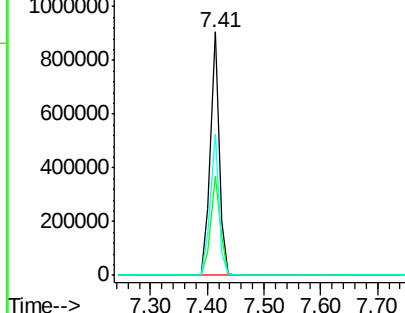
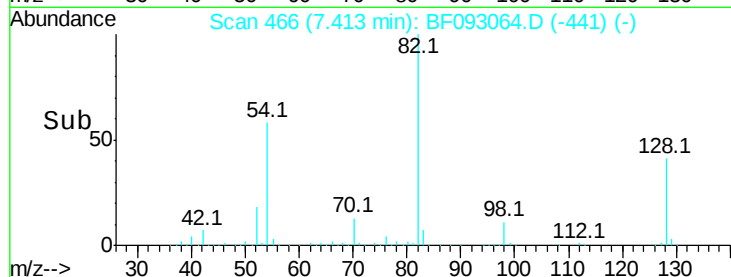


#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.89 min Scan# 683
 Delta R.T. -0.00 min
 Lab File: BF093064.D
 Acq: 21 Feb 2017 9:30

Tgt Ion	164	Resp	274771
Ion Ratio	Lower	Upper	
164	100		
162	107.6	80.2	120.2
160	48.4	36.9	55.3

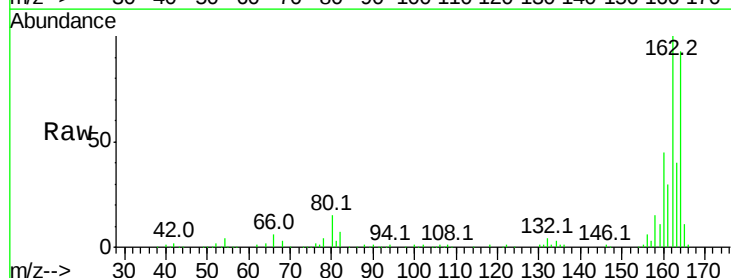

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

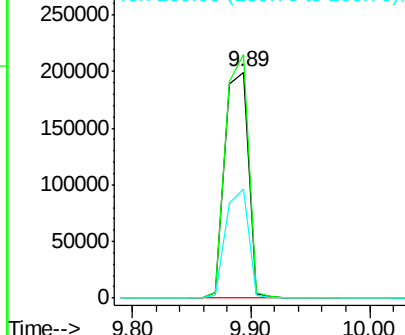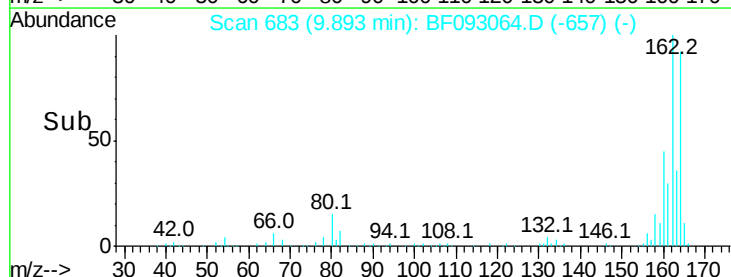






#41
 2,4,6-Tribromophenol
 Concen: 111.83 ng
 RT: 10.68 min Scan# 752
 Delta R.T. -0.00 min
 Lab File: BF093064.D
 Acq: 21 Feb 2017 9:30

Instrument :
 BNA_F
 ClientSampleId :
 021417-PRRT-F-D-S

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.3	77.4	116.2
141	34.6	34.1	51.1

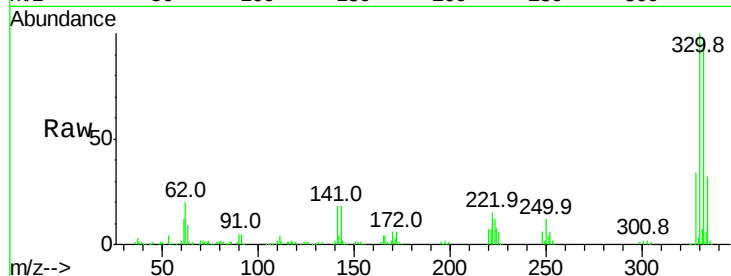


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

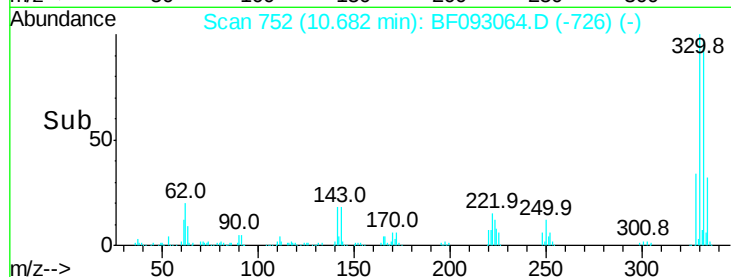
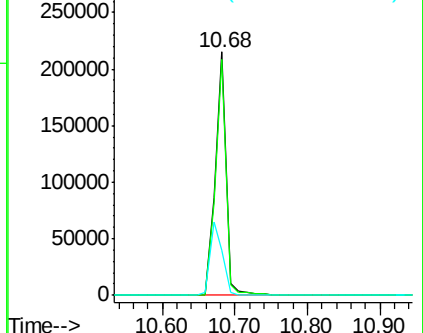



#44
 2-Fluorobiphenyl
 Concen: 119.01 ng
 RT: 9.22 min Scan# 624
 Delta R.T. -0.00 min
 Lab File: BF093064.D
 Acq: 21 Feb 2017 9:30

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.9	29.4	44.0
170	24.2	20.2	30.4

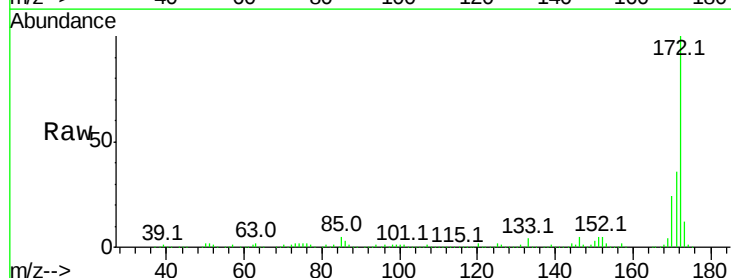

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



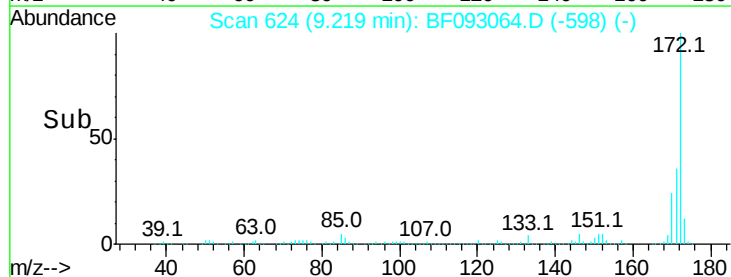
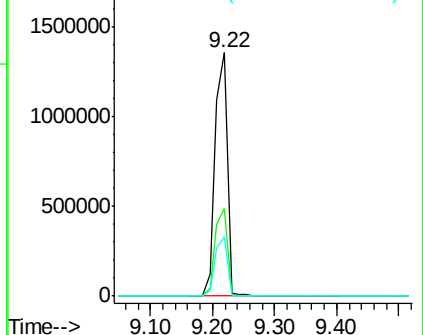


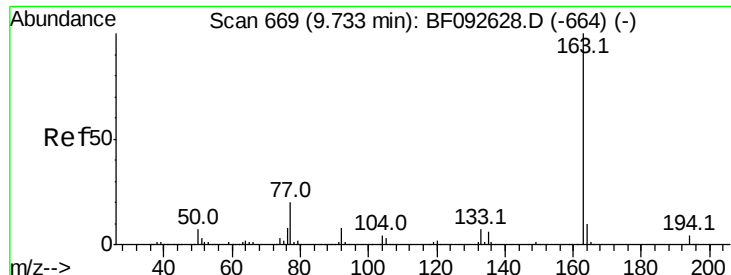

#49
Dimethylphthalate
Concen: 4.40 ng
RT: 9.61 min Scan# 658
Delta R.T. -0.01 min
Lab File: BF093064.D
Acq: 21 Feb 2017 9:30




Instrument :
BNA_F
ClientSampleId :
021417-PRRT-F-D-S


Tot Ion:163 Resp: 81382
Ion Ratio Lower Upper
163 100
194 3.3 3.0 4.4
164 10.1 8.0 12.0

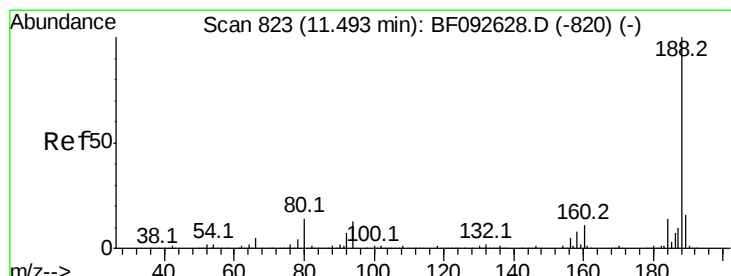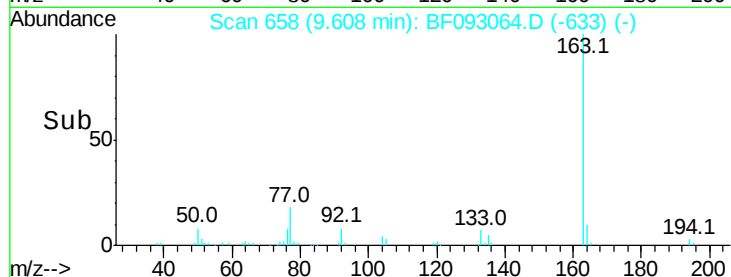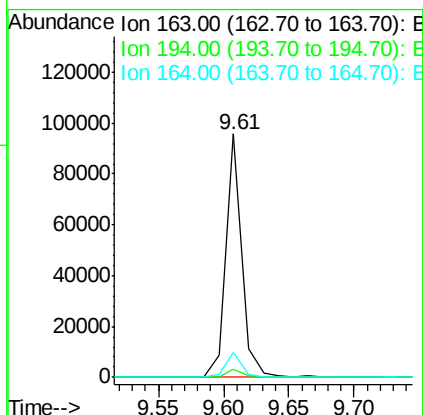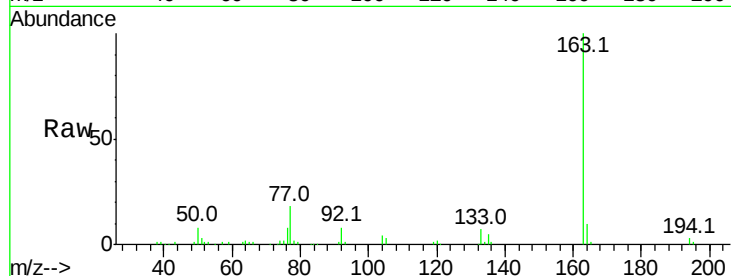

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.37 min Scan# 812
Delta R.T. -0.01 min
Lab File: BF093064.D
Acq: 21 Feb 2017 9:30

Tgt Ion:188 Resp: 476248
Ion Ratio Lower Upper
188 100
94 13.7 10.0 15.0
80 15.0 11.2 16.8

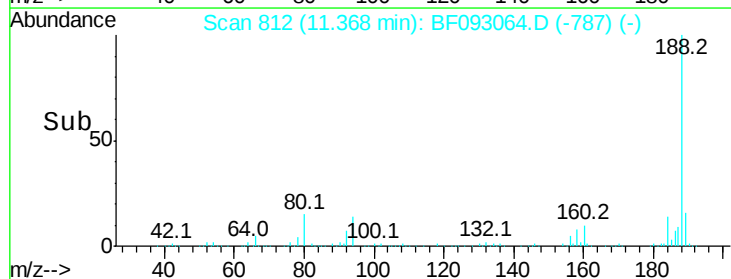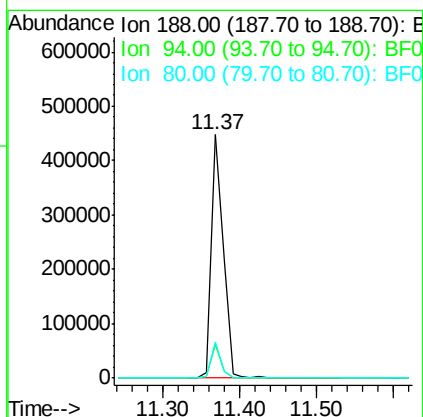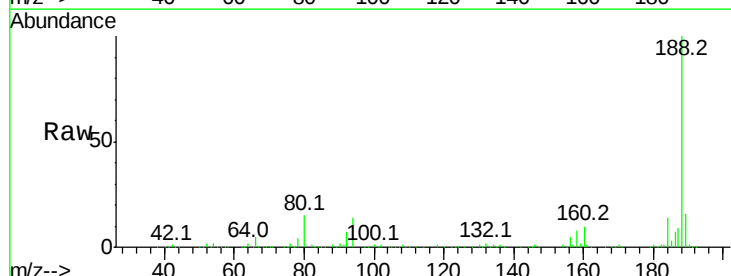

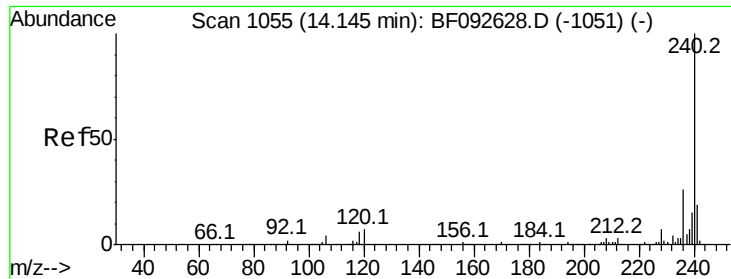

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.01 min Scan# 1043

Delta R.T. -0.01 min

Lab File: BF093064.D

Acq: 21 Feb 2017 9:30

Instrument :

BNA_F

ClientSampleId :

021417-PRRT-F-D-S


Tot Ion:240 Resp: 324587

Ion Ratio Lower Upper

240 100

120 9.8 12.9 19.3#




236 26.4 20.9 31.3

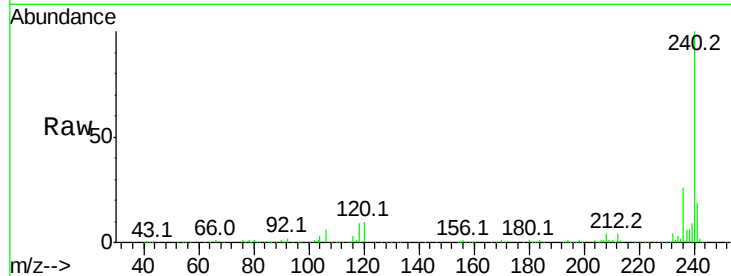

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

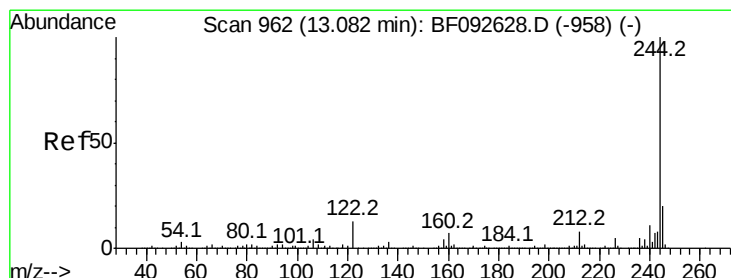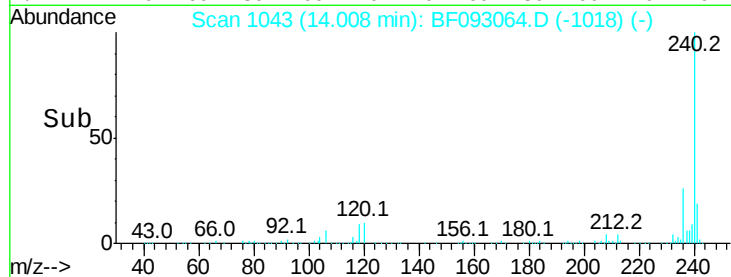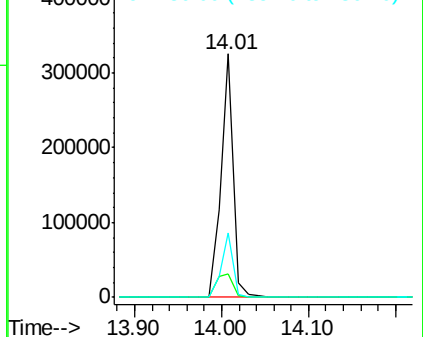

#78

Terphenyl-d14

Concen: 86.07 ng

RT: 12.96 min Scan# 951

Delta R.T. -0.01 min

Lab File: BF093064.D

Acq: 21 Feb 2017 9:30


Tgt Ion:244 Resp: 1189029

Ion Ratio Lower Upper

244 100

212 7.7 6.2 9.2



122 14.2 11.4 17.2

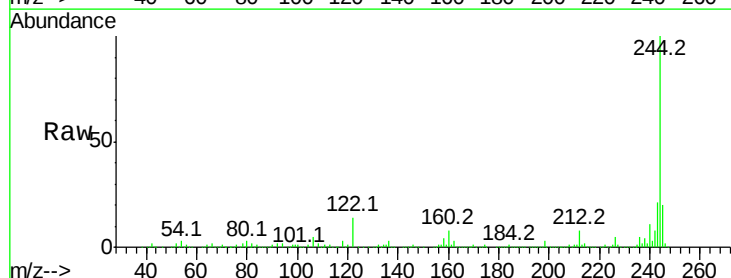


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

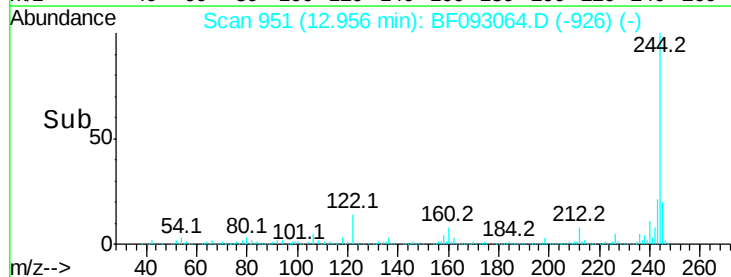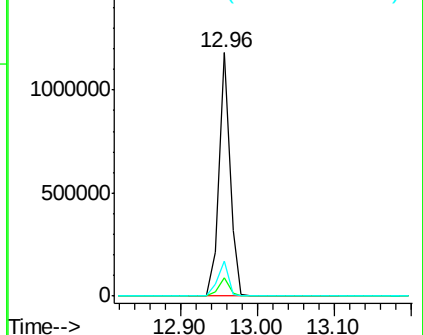

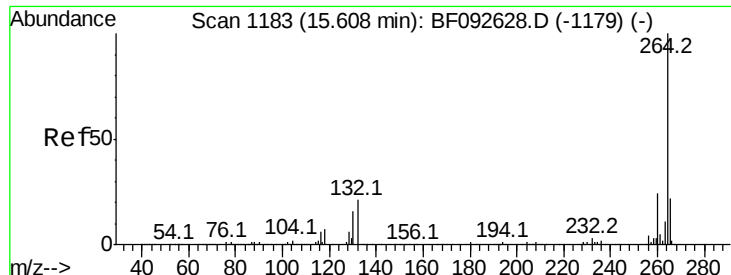

#86

Pervlene-d12

Concen: 20.00 ng

RT: 15.44 min Scan# 1168

Delta R.T. -0.01 min

Lab File: BF093064.D

Acq: 21 Feb 2017 9:30

Instrument :

BNA_F

ClientSampleId :

021417-PRRT-F-D-S


Tot Ion:264 Resp: 295185

Ion Ratio Lower Upper

264 100

260 23.8 19.2 28.8

265 21.0 17.4 26.0

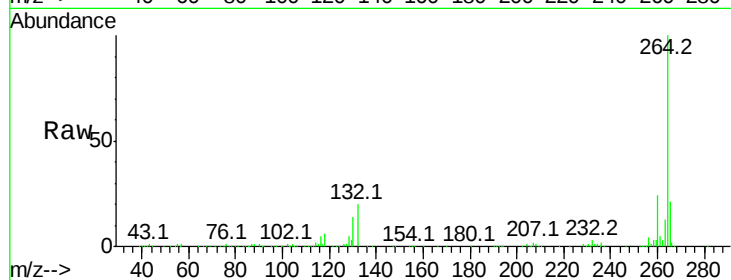

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

