


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF022017\
 Data File : BF093029.D
 Acq On : 20 Feb 2017 15:00
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 17 17:31:55 2017

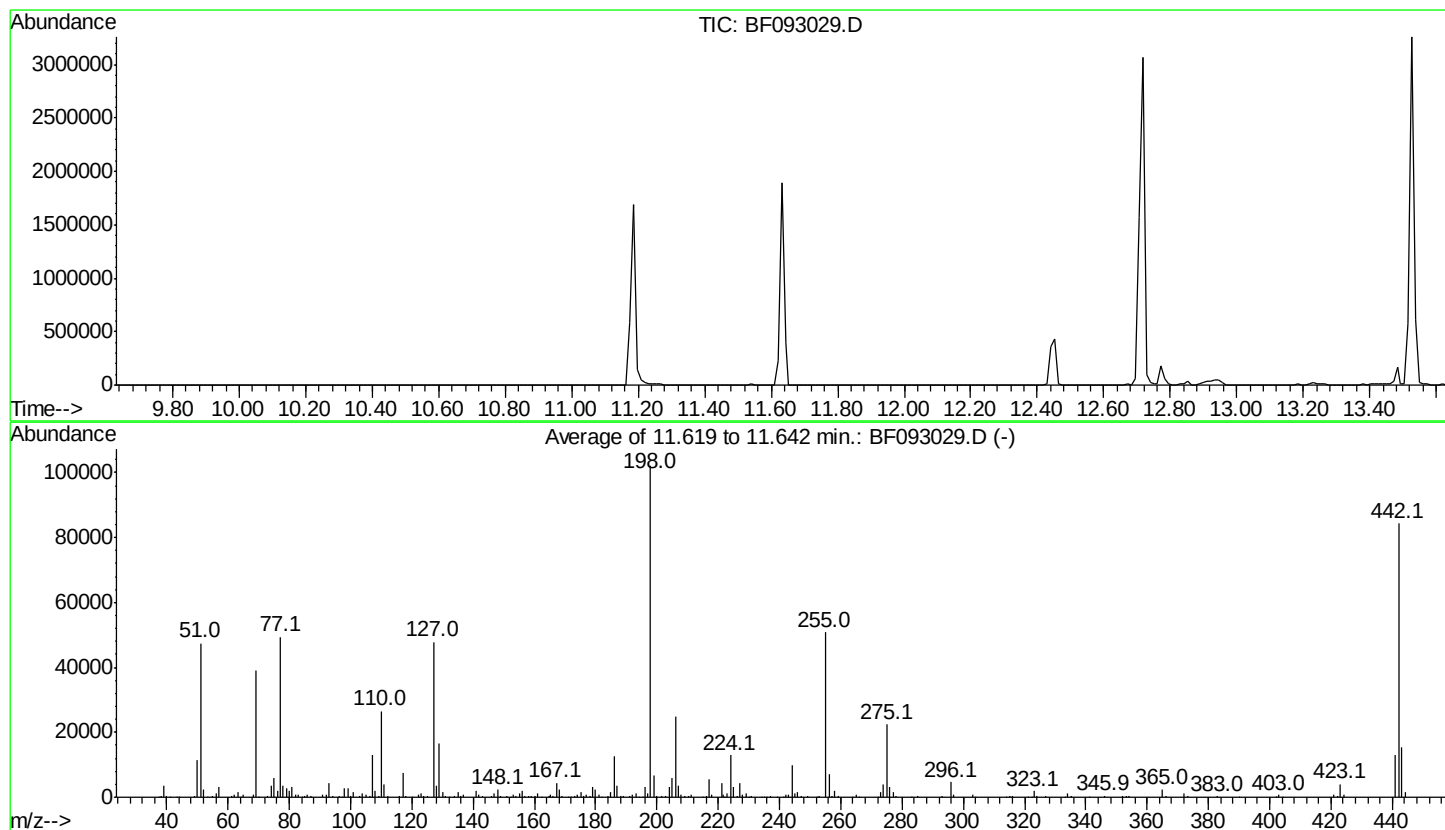

AutoFind: Scans 834, 835, 836; Background Corrected with Scan 831

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.3	47340	PASS
68	69	0.00	2	2.0	773	PASS
69	198	0.00	100	38.0	38863	PASS
70	69	0.00	2	0.4	154	PASS
127	198	10	80	46.7	47742	PASS
197	198	0.00	2	1.2	1177	PASS
198	198	100	100	100.0	102162	PASS
199	198	5	9	6.5	6680	PASS
275	198	10	60	22.0	22457	PASS
365	198	1	100	2.2	2274	PASS
441	442	0.01	24	15.6	13160	PASS
442	198	50	100	82.5	84235	PASS
443	442	15	24	18.3	15408	PASS