


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF022018\
 Data File : BF103111.D
 Acq On : 20 Feb 2018 8:42
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 16 14:34:49 2018

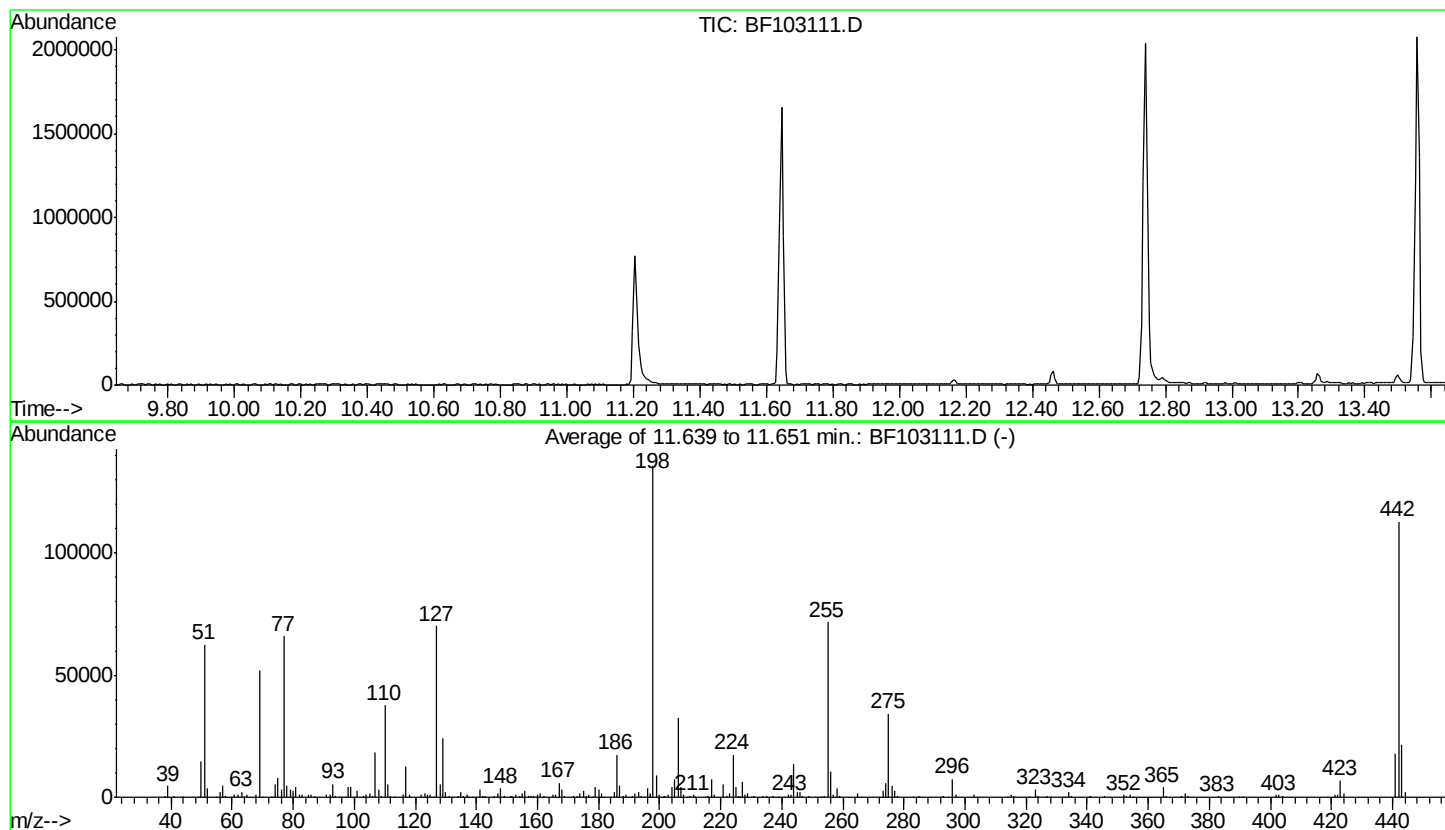

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	62603	PASS
68	69	0.00	2	1.8	921	PASS
69	198	0.00	100	38.0	51674	PASS
70	69	0.00	2	0.2	103	PASS
127	198	10	80	51.6	70053	PASS
197	198	0.00	2	1.0	1418	PASS
198	198	100	100	100.0	135808	PASS
199	198	5	9	6.7	9079	PASS
275	198	10	60	25.2	34253	PASS
365	198	1	100	2.9	3965	PASS
441	443	0.01	100	82.2	17706	PASS
442	198	50	100	83.1	112890	PASS
443	442	15	24	19.1	21529	PASS