
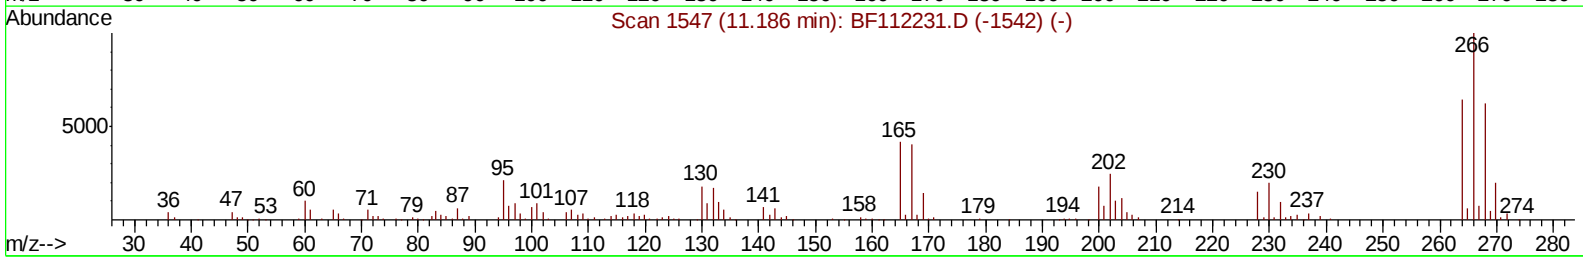
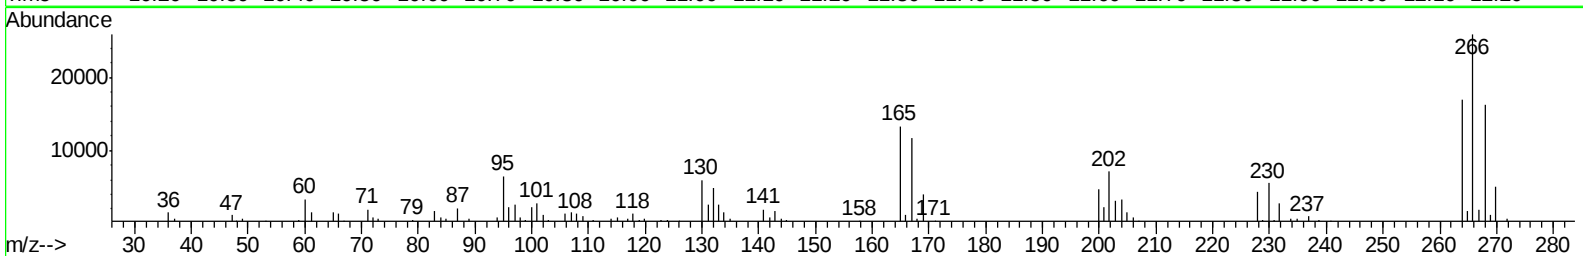


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022019\
Data File : BF112635.D
Acq On : 20 Feb 2019 11:59
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 05:29:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

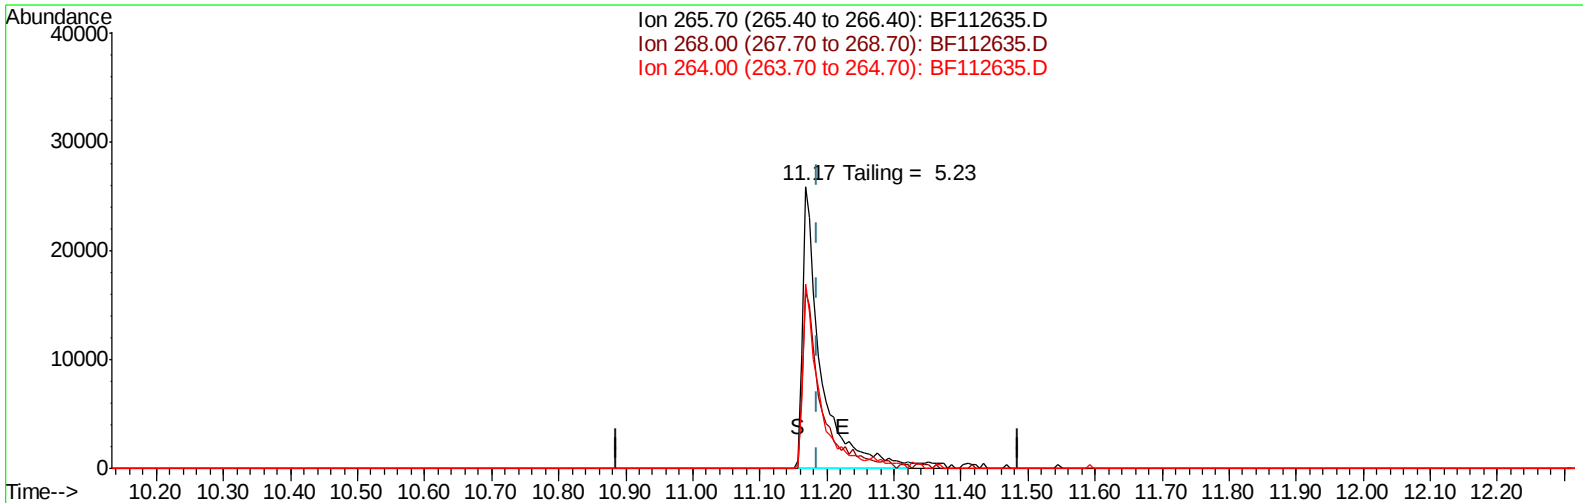

TIC: BF112635.D

(70) Pentachlorophenol (C)




11.169min (-0.018) 27744.30ng

response 48087

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	62.63
264.00	63.60	65.28
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022019\  
Data File : BF112635.D  
Acq On    : 20 Feb 2019   11:59  
Operator  : JU/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Feb 21 05:29:53 2019
Quant Method : Z:\SV0ASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

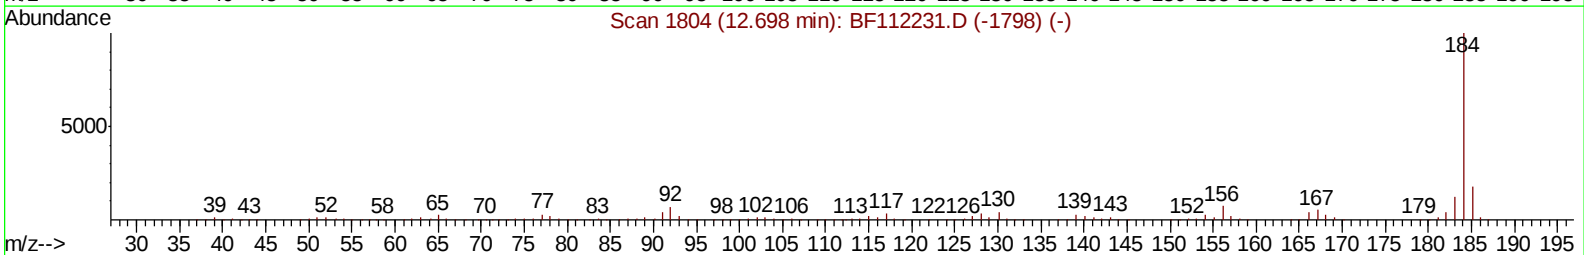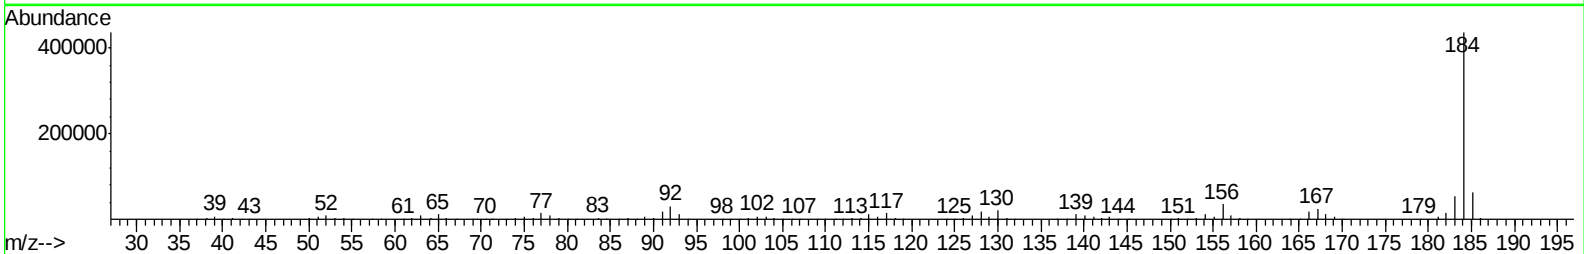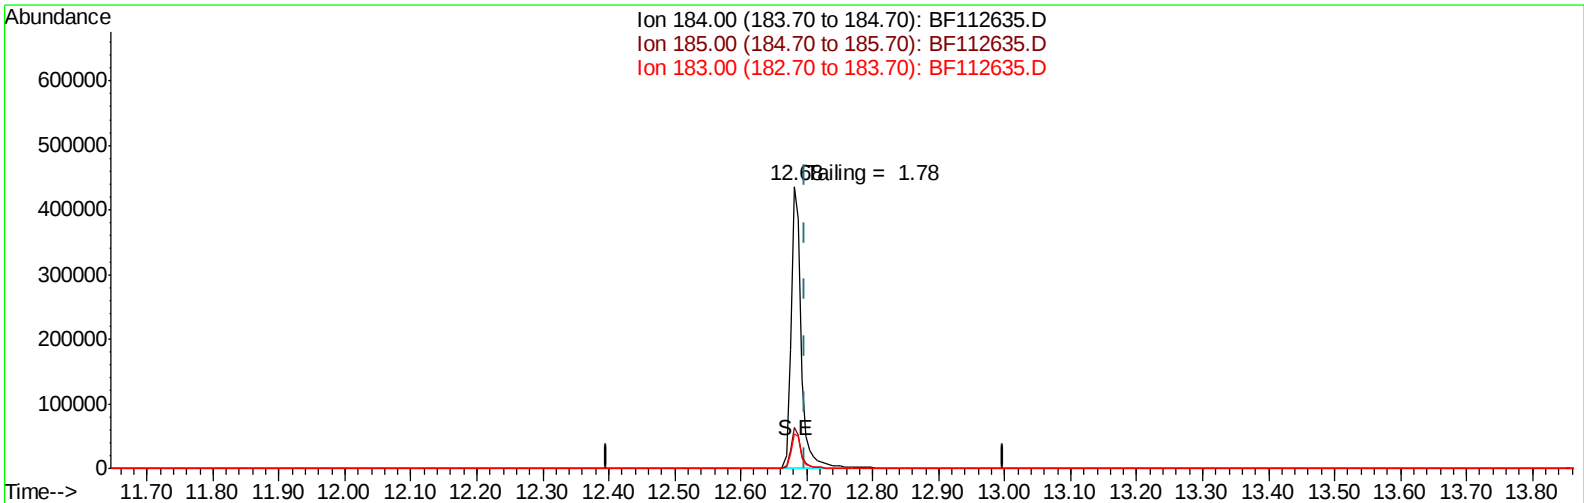

TIC: BF112635.D

(77) Benzidine

12.680min (-0.018) 0.00ng

response 468987

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	14.53
183.00	12.50	12.46
0.00	0.00	0.00