


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022019\
 Data File : BF112635.D
 Acq On : 20 Feb 2019 11:59
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 28 10:38:18 2019

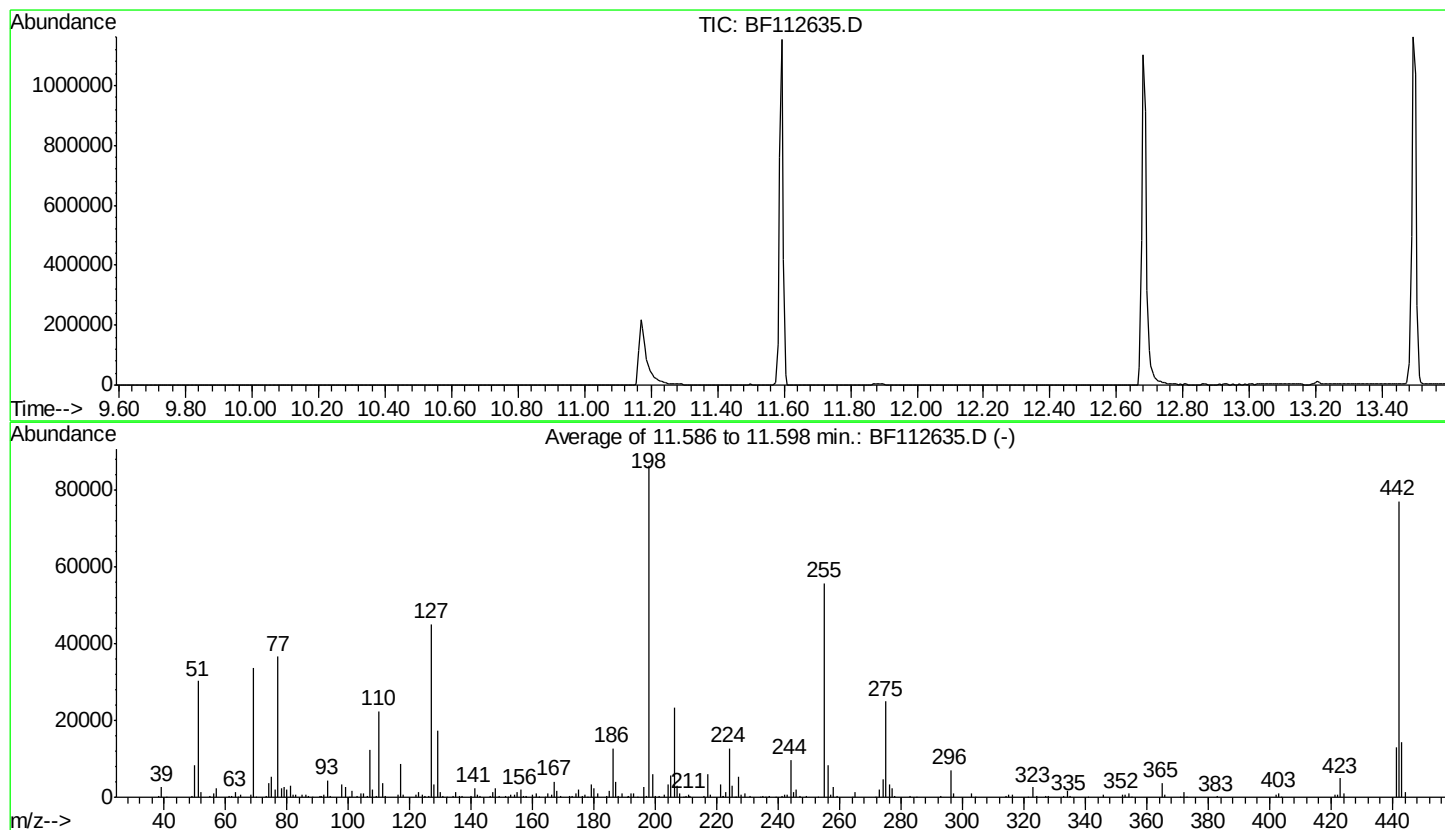

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	30202	PASS
68	69	0.00	2	1.9	638	PASS
69	198	0.00	100	38.8	33521	PASS
70	69	0.00	2	0.4	141	PASS
127	198	10	80	52.1	45024	PASS
197	198	0.00	2	0.2	183	PASS
198	198	100	100	100.0	86352	PASS
199	198	5	9	6.8	5860	PASS
275	198	10	60	28.9	24916	PASS
365	198	1	100	4.3	3709	PASS
441	198	0.01	100	14.9	12868	PASS
442	198	50	100	89.3	77141	PASS
443	442	15	24	18.4	14192	PASS