
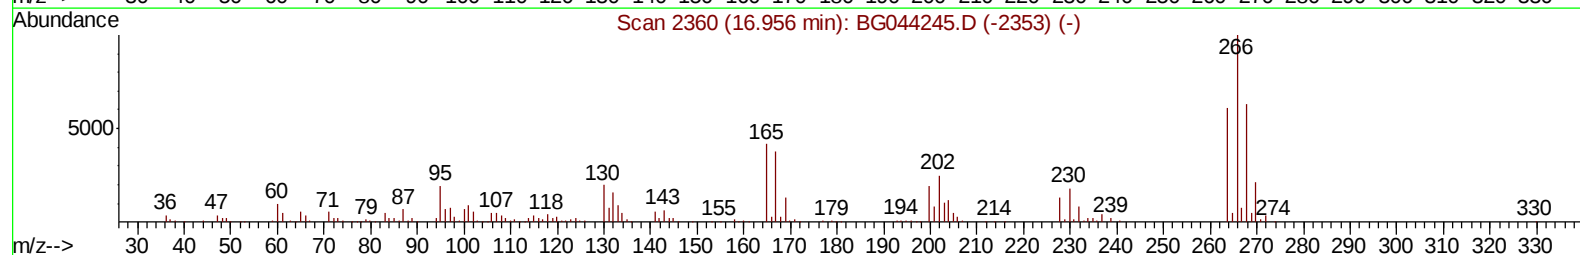
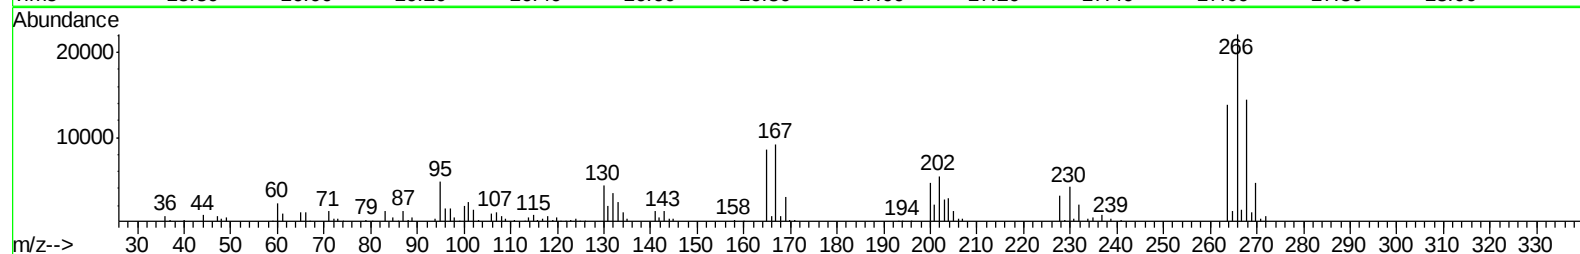


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG022020\
Data File : BG044516.D
Acq On : 20 Feb 2020 11:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 08:09:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 10 16:11:50 2020
Response via : Initial Calibration

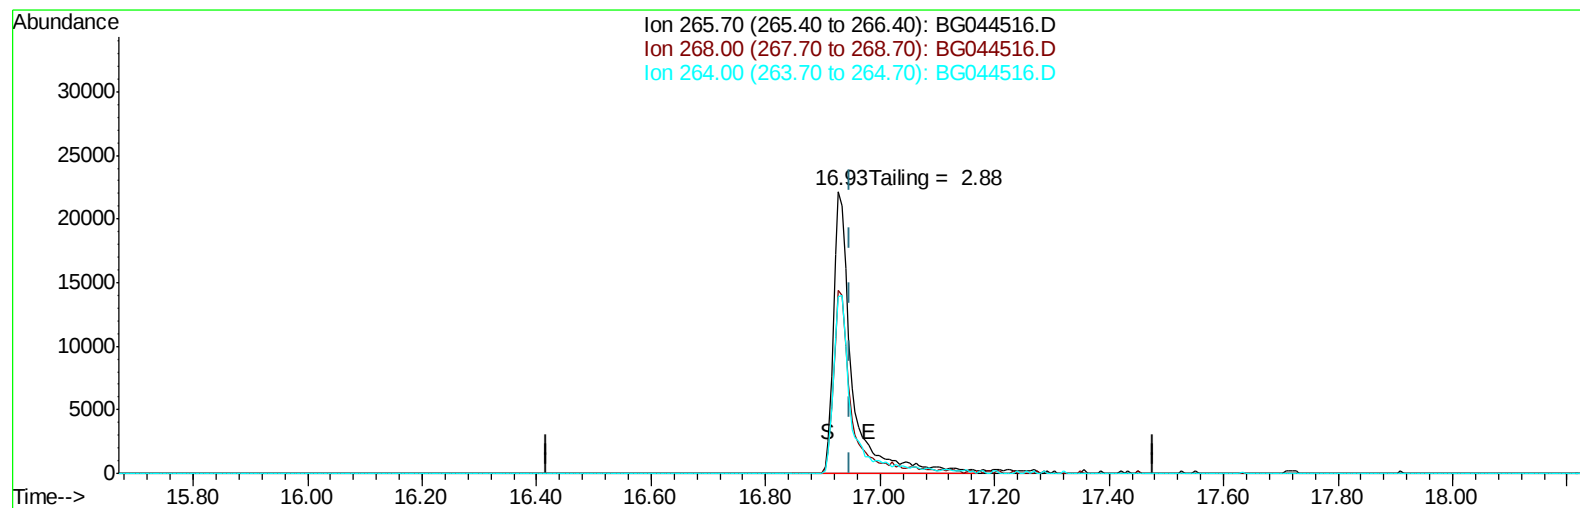

TIC: BG044516.D

(70) Pentachlorophenol (C)




16.927min (-0.020) 28497.44ng

response 46499

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	65.02
264.00	60.90	62.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG022020\
 Data File : BG044516.D
 Acq On : 20 Feb 2020 11:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 08:09:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 10 16:11:50 2020
 Response via : Initial Calibration

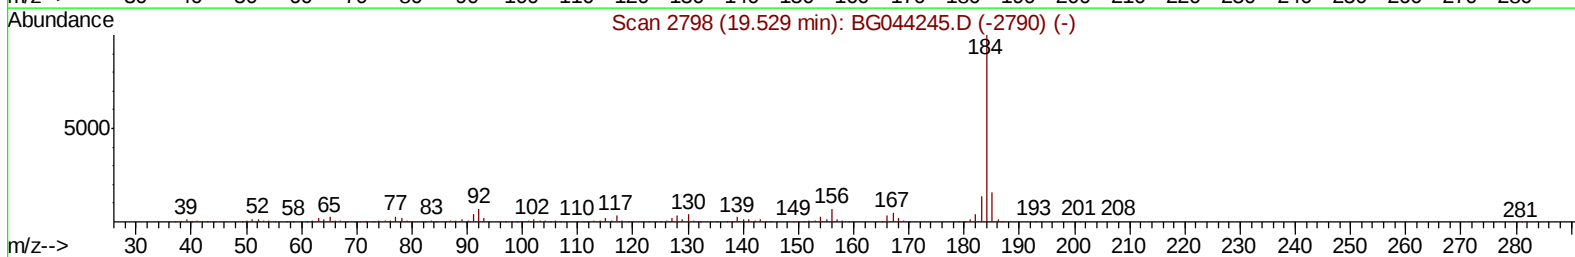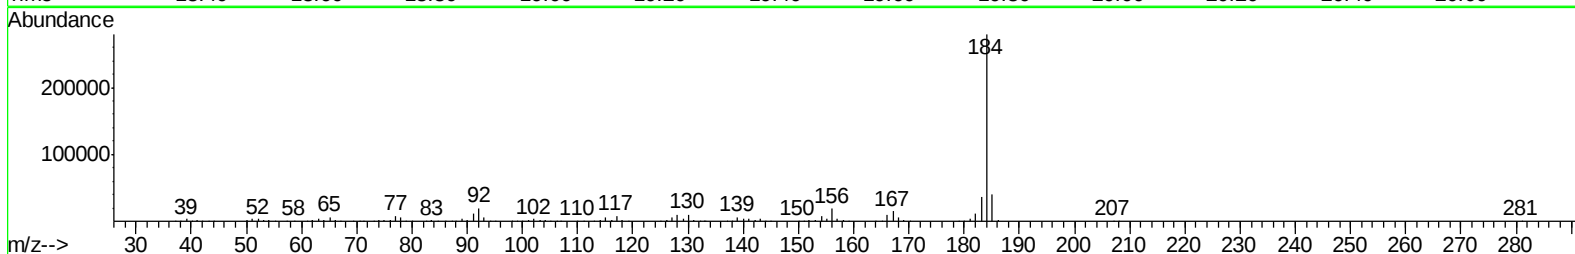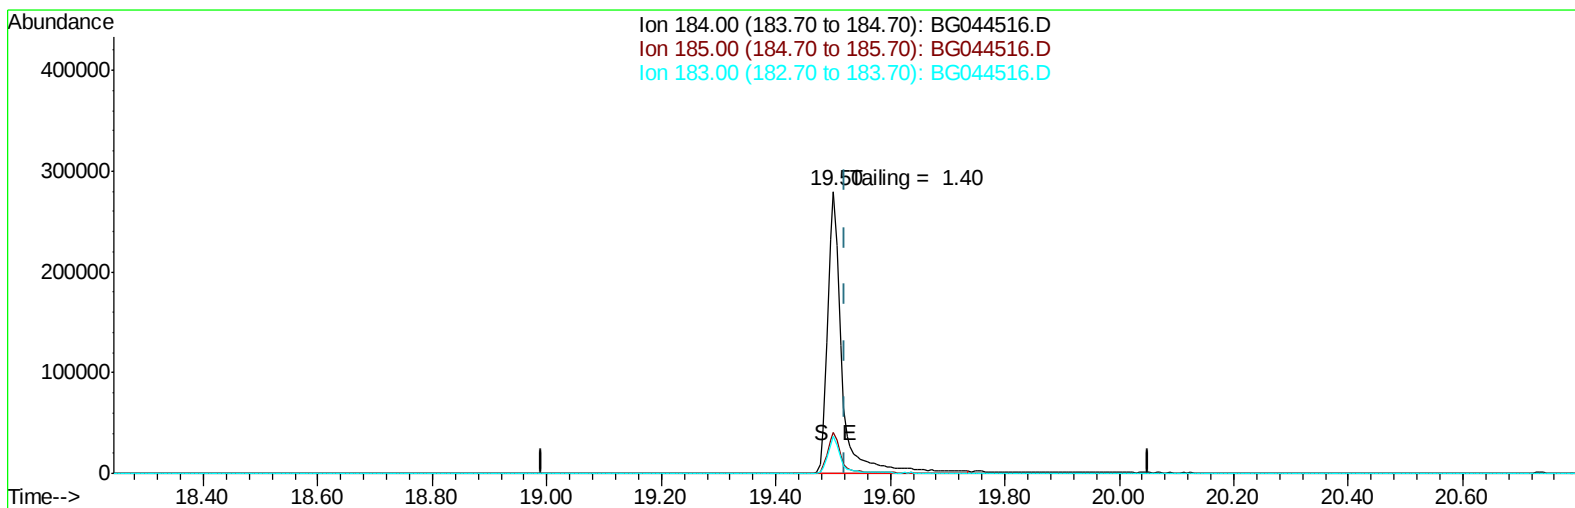

TIC: BG044516.D

(77) Benzidine

19.501min (-0.020) 0.00ng

response 484174

Ion	Exp%	Act%
184.00	100	100
185.00	16.10	14.50
183.00	13.50	12.98
0.00	0.00	0.00