

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022020\
 Data File : BF118981.D
 Acq On : 21 Feb 2020 1:59
 Operator : CG/JU
 Sample : L1468-05DL 50X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP9-EP1-2.5DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.757	791	794	798	rBV	1391796	1133620	26.00%	2.266%
2	6.940	822	825	829	rVB	493977	400308	9.18%	0.800%
3	7.022	835	839	845	rBV	89590	89522	2.05%	0.179%
4	7.792	965	970	973	rBV3	76414	95093	2.18%	0.190%
5	7.828	973	976	984	rVB2	74315	121484	2.79%	0.243%
6	8.039	1008	1012	1014	rBV	1623236	1793776	41.14%	3.586%
7	8.063	1014	1016	1020	rVV	4615590	4359846	100.00%	8.715%
8	8.110	1021	1024	1029	rVB	195646	179008	4.11%	0.358%
9	8.751	1129	1133	1137	rBV	1596920	1331556	30.54%	2.662%
10	8.851	1145	1150	1153	rBV	954000	784397	17.99%	1.568%
11	9.110	1191	1194	1198	rVB	138569	109199	2.50%	0.218%
12	9.210	1208	1211	1218	rVB	312700	287186	6.59%	0.574%
13	9.310	1225	1228	1234	rVB	133886	143482	3.29%	0.287%
14	9.381	1234	1240	1243	rBV	248470	330721	7.59%	0.661%
15	9.451	1248	1252	1254	rVV	378577	360163	8.26%	0.720%
16	9.475	1254	1256	1260	rVV	223893	219379	5.03%	0.439%
17	9.569	1266	1272	1281	rBV	166495	197865	4.54%	0.396%
18	9.651	1281	1286	1290	rBV	542605	442585	10.15%	0.885%
19	9.792	1303	1310	1312	rVV	2042578	1829924	41.97%	3.658%
20	9.822	1312	1315	1319	rVV	1054085	870199	19.96%	1.739%
21	9.992	1340	1344	1348	rVV	880665	770283	17.67%	1.540%
22	10.033	1348	1351	1354	rVB	96321	78300	1.80%	0.157%
23	10.104	1359	1363	1366	rBV3	89858	109763	2.52%	0.219%
24	10.198	1374	1379	1381	rBV2	64066	88972	2.04%	0.178%
25	10.239	1384	1386	1389	rVB	85788	70682	1.62%	0.141%
26	10.339	1399	1403	1409	rVV	1449326	1330252	30.51%	2.659%
27	10.445	1419	1421	1426	rVV2	104647	116532	2.67%	0.233%
28	10.492	1426	1429	1432	rVV	201933	193266	4.43%	0.386%
29	10.557	1436	1440	1441	rVV	192524	161186	3.70%	0.322%
30	10.575	1441	1443	1447	rVV	258505	278312	6.38%	0.556%
31	10.704	1461	1465	1470	rVB2	72105	89678	2.06%	0.179%
32	10.886	1488	1496	1498	rBV2	181369	246591	5.66%	0.493%
33	10.910	1498	1500	1504	rVV	100177	95674	2.19%	0.191%
34	10.969	1507	1510	1513	rVV2	94153	99865	2.29%	0.200%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022020\
 Data File : BF118981.D
 Acq On : 21 Feb 2020 1:59
 Operator : CG/JU
 Sample : L1468-05DL 50X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP9-EP1-2.5DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.033	1519	1521	1527	rVV2	71518	95455	2.19%	0.191%
36	11.122	1533	1536	1539	rVV2	62072	70579	1.62%	0.141%
37	11.169	1539	1544	1551	rVB	423118	440086	10.09%	0.880%
38	11.275	1558	1562	1564	rBV	1696181	1754585	40.24%	3.507%
39	11.298	1564	1566	1570	rVV	4035850	3671355	84.21%	7.339%
40	11.351	1570	1575	1578	rVV	1403366	1297145	29.75%	2.593%
41	11.380	1578	1580	1584	rVB	135329	130372	2.99%	0.261%
42	11.504	1595	1601	1604	rBV	475121	493515	11.32%	0.986%
43	11.569	1609	1612	1615	rVV2	149972	137463	3.15%	0.275%
44	11.604	1615	1618	1623	rVB2	133074	139424	3.20%	0.279%
45	11.686	1629	1632	1636	rVB	98701	114345	2.62%	0.229%
46	11.775	1643	1647	1649	rBV	435480	393934	9.04%	0.787%
47	11.804	1649	1652	1655	rVB	555227	514156	11.79%	1.028%
48	11.851	1656	1660	1662	rBV	199906	174623	4.01%	0.349%
49	11.886	1662	1666	1668	rVV	827642	818156	18.77%	1.635%
50	11.904	1668	1669	1674	rVB	261503	224686	5.15%	0.449%
51	11.975	1679	1681	1684	rVB	84027	72462	1.66%	0.145%
52	12.069	1694	1697	1700	rBV	275941	235753	5.41%	0.471%
53	12.251	1725	1728	1730	rBV	70699	76434	1.75%	0.153%
54	12.322	1737	1740	1743	rBV	210979	223054	5.12%	0.446%
55	12.363	1743	1747	1749	rVV2	144294	195088	4.47%	0.390%
56	12.416	1752	1756	1759	rVV3	59149	97126	2.23%	0.194%
57	12.486	1764	1768	1771	rBV	2883853	2545722	58.39%	5.089%
58	12.574	1781	1783	1787	rVB	373859	355365	8.15%	0.710%
59	12.633	1787	1793	1800	rVB3	131944	218286	5.01%	0.436%
60	12.716	1800	1807	1810	rBV2	2149849	2446030	56.10%	4.889%
61	12.763	1812	1815	1820	rVB2	121839	143745	3.30%	0.287%
62	12.827	1823	1826	1828	rBV	143790	146097	3.35%	0.292%
63	12.851	1828	1830	1832	rVV	128470	115549	2.65%	0.231%
64	12.869	1832	1833	1839	rVB	105579	92357	2.12%	0.185%
65	12.933	1839	1844	1846	rBV2	160262	260918	5.98%	0.522%
66	13.016	1854	1858	1859	rVV4	135398	159316	3.65%	0.318%
67	13.039	1859	1862	1865	rVB	548180	500115	11.47%	1.000%
68	13.104	1865	1873	1876	rBV	584127	567564	13.02%	1.134%
69	13.145	1876	1880	1883	rVV2	218487	247451	5.68%	0.495%
70	13.210	1887	1891	1893	rBV3	83246	120353	2.76%	0.241%
71	13.233	1893	1895	1898	rVV	143156	131701	3.02%	0.263%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022020\
 Data File : BF118981.D
 Acq On : 21 Feb 2020 1:59
 Operator : CG/JU
 Sample : L1468-05DL 50X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP9-EP1-2.5DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	13.263	1898	1900	1905	rVB	150470	170148	3.90%	0.340%
73	13.521	1940	1944	1947	rBV2	72490	92520	2.12%	0.185%
74	13.657	1961	1967	1969	rBV	185788	227512	5.22%	0.455%
75	13.686	1969	1972	1974	rVV	186010	199972	4.59%	0.400%
76	13.710	1974	1976	1983	rVB3	137071	205228	4.71%	0.410%
77	13.904	2002	2009	2012	rBV2	2101007	2891706	66.33%	5.780%
78	13.933	2012	2014	2021	rVB	1121631	962685	22.08%	1.924%
79	14.051	2032	2034	2037	rBV	73507	73415	1.68%	0.147%
80	14.098	2039	2042	2044	rVB	91648	78524	1.80%	0.157%
81	14.133	2044	2048	2051	rBV2	101995	123781	2.84%	0.247%
82	14.292	2071	2075	2078	rVV	191700	195725	4.49%	0.391%
83	14.327	2078	2081	2084	rVB	111829	96732	2.22%	0.193%
84	14.386	2085	2091	2094	rBV3	133626	204414	4.69%	0.409%
85	14.416	2094	2096	2098	rVV	124407	126276	2.90%	0.252%
86	14.439	2098	2100	2103	rVV2	182986	159674	3.66%	0.319%
87	14.486	2105	2108	2114	rVB3	88437	90600	2.08%	0.181%
88	14.833	2164	2167	2172	rBV5	50892	78932	1.81%	0.158%
89	14.927	2178	2183	2192	rBV	732111	1458508	33.45%	2.915%
90	14.998	2192	2195	2197	rVV2	78692	88216	2.02%	0.176%
91	15.027	2197	2200	2205	rVB	208121	234620	5.38%	0.469%
92	15.215	2228	2232	2238	rVB	429440	525636	12.06%	1.051%
93	15.274	2238	2242	2247	rBV	771389	869660	19.95%	1.738%
94	15.333	2247	2252	2255	rBV	1105296	1376517	31.57%	2.751%
95	15.868	2340	2343	2348	rVB2	63342	93687	2.15%	0.187%
96	16.015	2364	2368	2374	rBV3	45479	81393	1.87%	0.163%
97	16.733	2484	2490	2497	rBV	261005	483263	11.08%	0.966%
98	16.898	2514	2518	2522	rBV	49317	82859	1.90%	0.166%
99	17.151	2556	2561	2571	rVB	176287	365371	8.38%	0.730%
100	17.380	2595	2600	2607	rBV	76768	161767	3.71%	0.323%


Sum of corrected areas: 50028375

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022020\
Data File : BF118981.D
Acq On : 21 Feb 2020 1:59
Operator : CG/JU
Sample : L1468-05DL 50X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP9-EP1-2.5DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

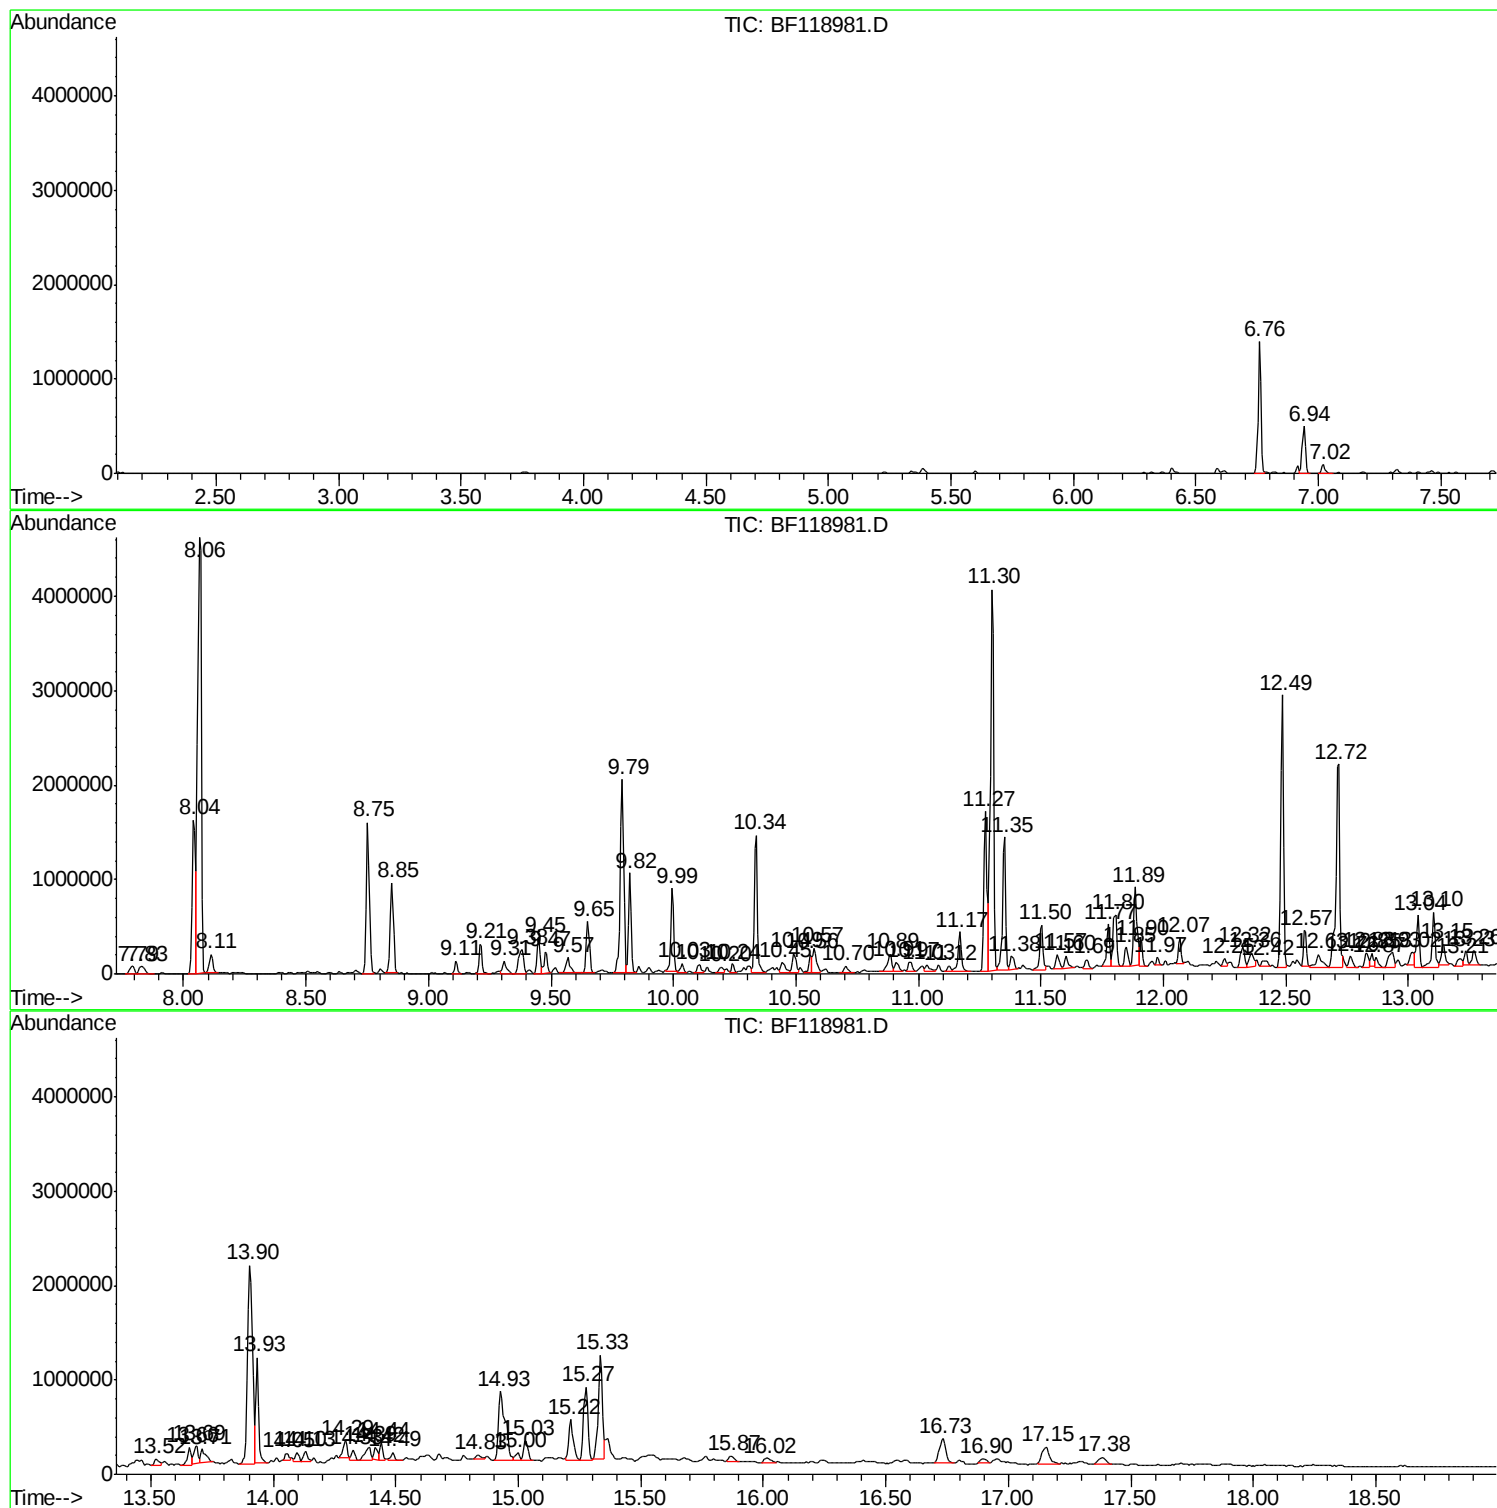

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022020\
Data_File : BF118981.D
Acq_On : 21_Feb_2020 1:59
Operator : CG/JUU
Sample : L1468-05DL_50XX
Misc :
ALS_Vial : 17 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
TP9-EP1-2.5DL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
