


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022020\
 Data File : BF118956.D
 Acq On : 20 Feb 2020 12:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 20 17:40:17 2020

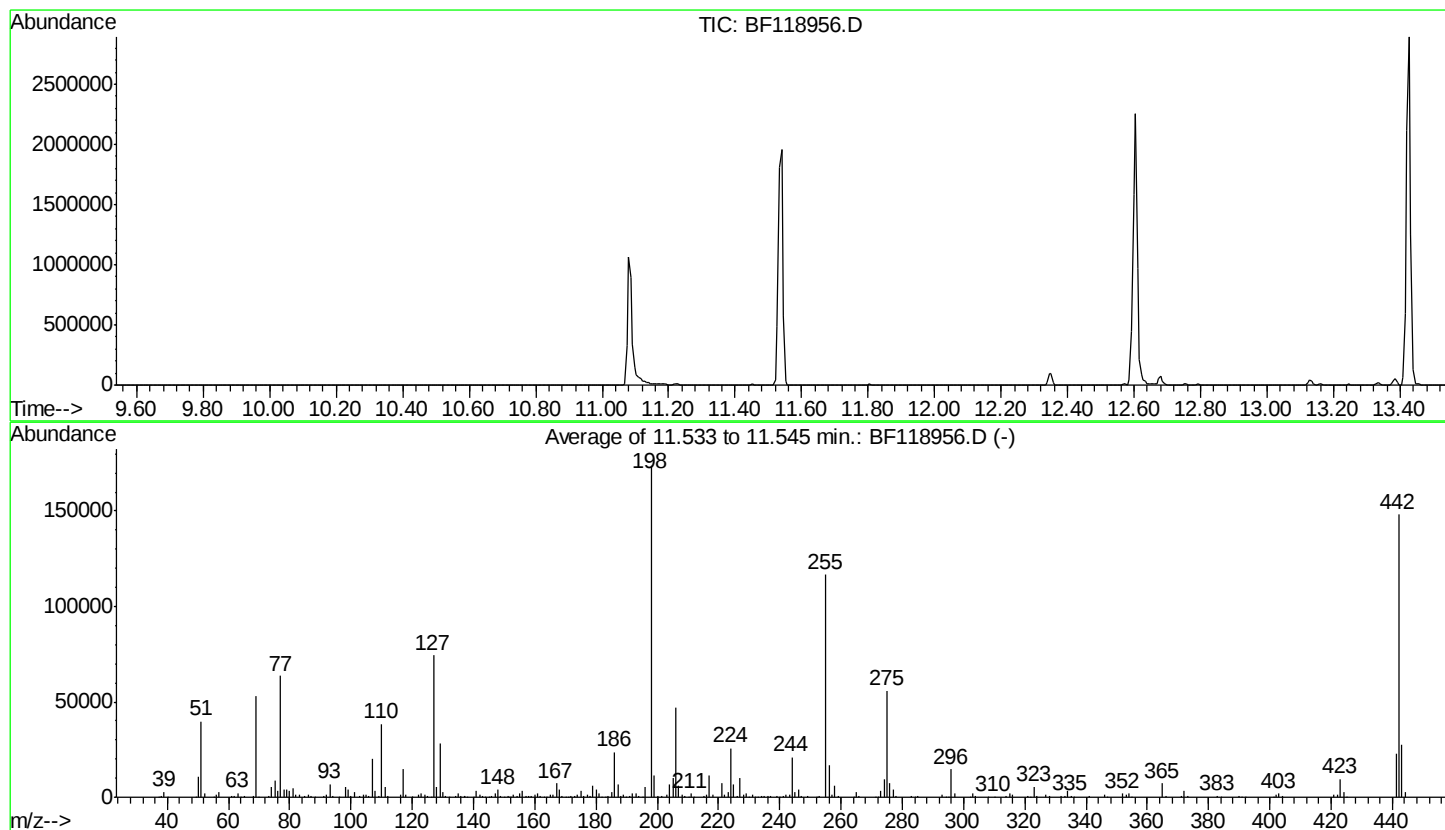

AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.8	39714	PASS
68	69	0.00	2	1.8	938	PASS
69	198	0.00	100	30.3	52718	PASS
70	69	0.00	2	0.5	278	PASS
127	198	10	80	42.8	74453	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	173821	PASS
199	198	5	9	6.6	11437	PASS
275	198	10	60	32.2	56050	PASS
365	198	1	100	4.2	7343	PASS
441	198	0.01	100	13.1	22768	PASS
442	198	50	100	85.2	148162	PASS
443	442	15	24	18.4	27210	PASS