


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022020\
 Data File : BF118965.D
 Acq On : 20 Feb 2020 18:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 20 17:40:17 2020

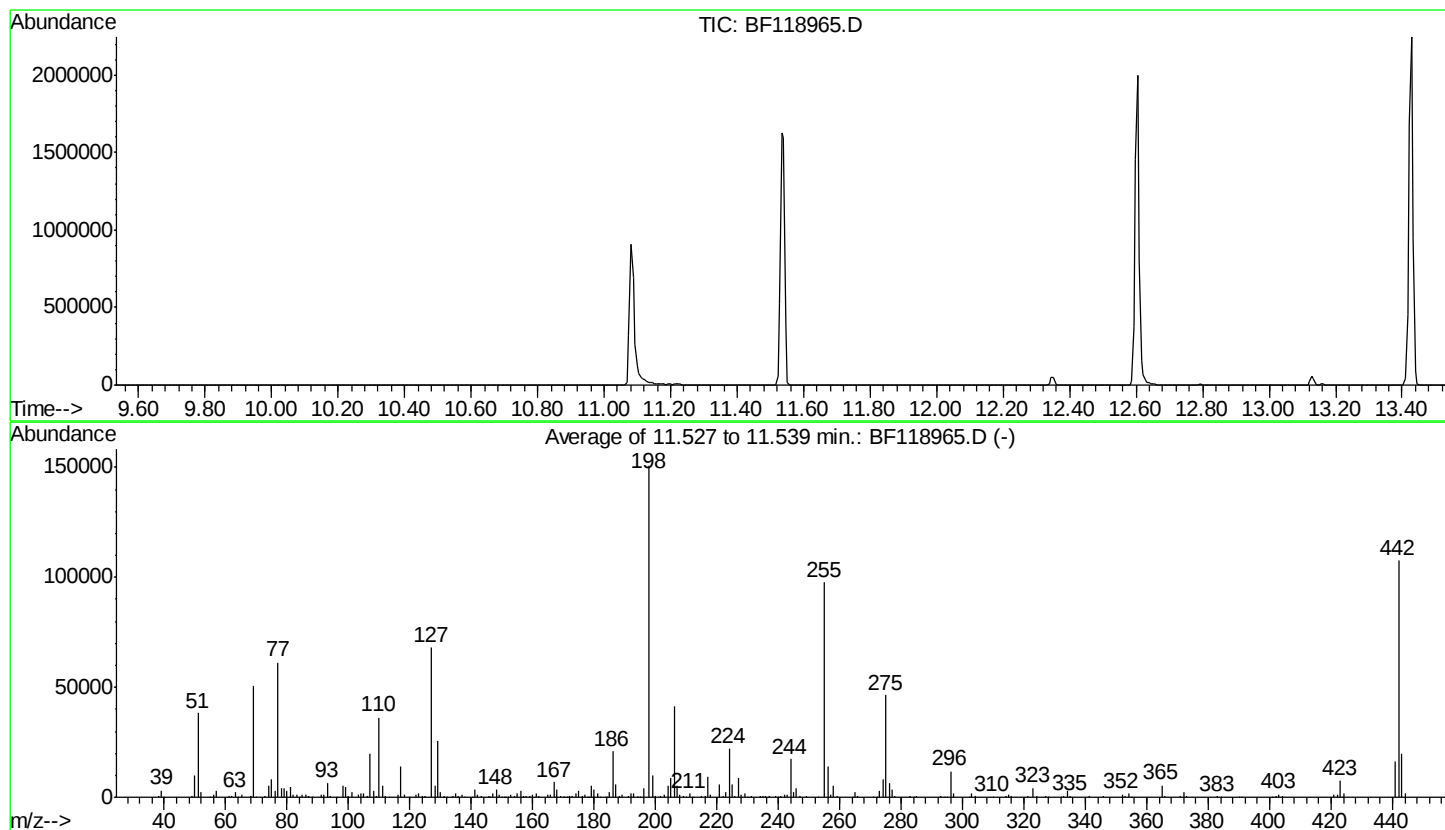

AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.4	38368	PASS
68	69	0.00	2	1.5	751	PASS
69	198	0.00	100	33.8	50962	PASS
70	69	0.00	2	0.3	166	PASS
127	198	10	80	45.2	68101	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	150824	PASS
199	198	5	9	6.7	10160	PASS
275	198	10	60	30.8	46428	PASS
365	198	1	100	3.7	5523	PASS
441	198	0.01	100	10.8	16256	PASS
442	198	50	100	71.3	107528	PASS
443	442	15	24	18.4	19830	PASS