

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
 Data File : BF141696.D
 Acq On : 20 Feb 2025 11:33
 Operator : RC/JU
 Sample : PB166772BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB166772BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141696.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.840	292	297	309	rBV	17919	31727	1.02%	0.174%
2	5.410	558	564	588	rBV	1859421	2594351	83.07%	14.235%
3	6.422	730	736	756	rBV	1773274	2555809	81.83%	14.024%
4	6.781	792	797	811	rVB	403501	529770	16.96%	2.907%
5	7.345	886	893	911	rBV	1177541	1698392	54.38%	9.319%
6	8.063	1009	1015	1033	rBV	466809	687581	22.02%	3.773%
7	9.134	1191	1197	1223	rBV	2342530	3123200	100.00%	17.137%
8	9.810	1307	1312	1335	rVB	543321	760605	24.35%	4.173%
9	10.604	1441	1447	1479	rBV	1197484	1699239	54.41%	9.324%
10	11.298	1560	1565	1584	rBV	514635	729767	23.37%	4.004%
11	12.880	1828	1834	1850	rBV	2165333	2868953	91.86%	15.742%
12	13.933	2008	2013	2028	rBV	331025	499520	15.99%	2.741%
13	15.380	2252	2259	2273	rBV	244510	446176	14.29%	2.448%




Sum of corrected areas: 18225090

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141696.D
Acq On : 20 Feb 2025 11:33
Operator : RC/JU
Sample : PB166772BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166772BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

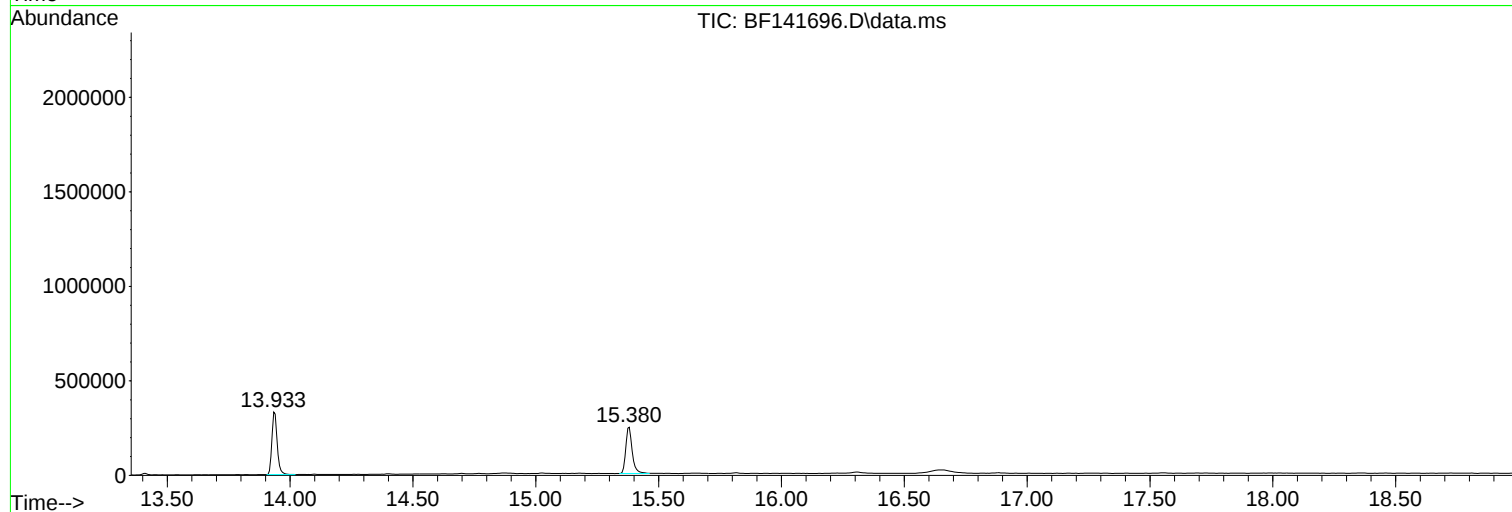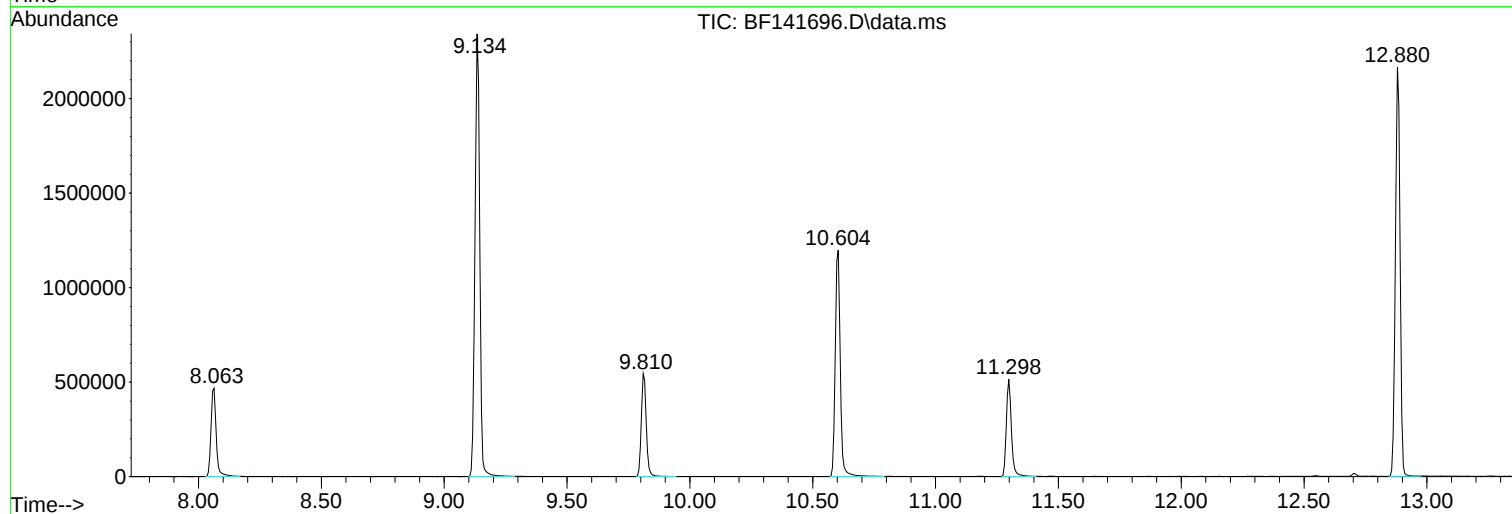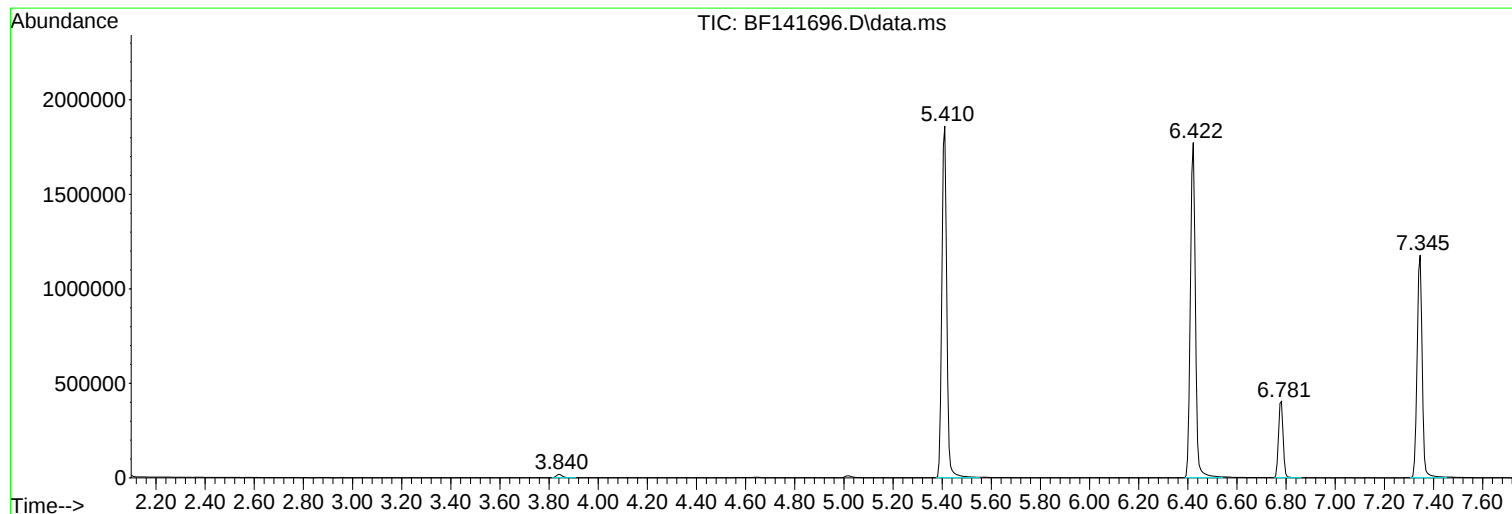

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141696.D
Acq On : 20 Feb 2025 11:33
Operator : RC/JU
Sample : PB166772BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166772BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141696.D
Acq On : 20 Feb 2025 11:33
Operator : RC/JU
Sample : PB166772BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166772BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------