

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141698.D
Acq On : 20 Feb 2025 12:33
Operator : RC/JU
Sample : PB166776BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166776BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141698.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.404	558	563	586	rBV	1761269	2507154	83.23%	14.196%
2	6.422	730	736	771	rBV	1730283	2480559	82.35%	14.045%
3	6.781	792	797	814	rVB	402613	521347	17.31%	2.952%
4	7.345	886	893	922	rBV	1151937	1641464	54.49%	9.294%
5	8.063	1009	1015	1034	rBV	462118	674372	22.39%	3.818%
6	9.133	1191	1197	1222	rBV	2270058	3012309	100.00%	17.056%
7	9.810	1307	1312	1332	rBV	530600	744793	24.72%	4.217%
8	10.604	1441	1447	1471	rBV	1137055	1648890	54.74%	9.336%
9	11.298	1559	1565	1586	rBV	492421	711383	23.62%	4.028%
10	12.880	1828	1834	1854	rBV	2127046	2774961	92.12%	15.712%
11	13.939	2008	2014	2026	rBV	328580	501429	16.65%	2.839%
12	15.380	2253	2259	2277	rVB	245754	442743	14.70%	2.507%




Sum of corrected areas: 17661404

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141698.D
Acq On : 20 Feb 2025 12:33
Operator : RC/JU
Sample : PB166776BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166776BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

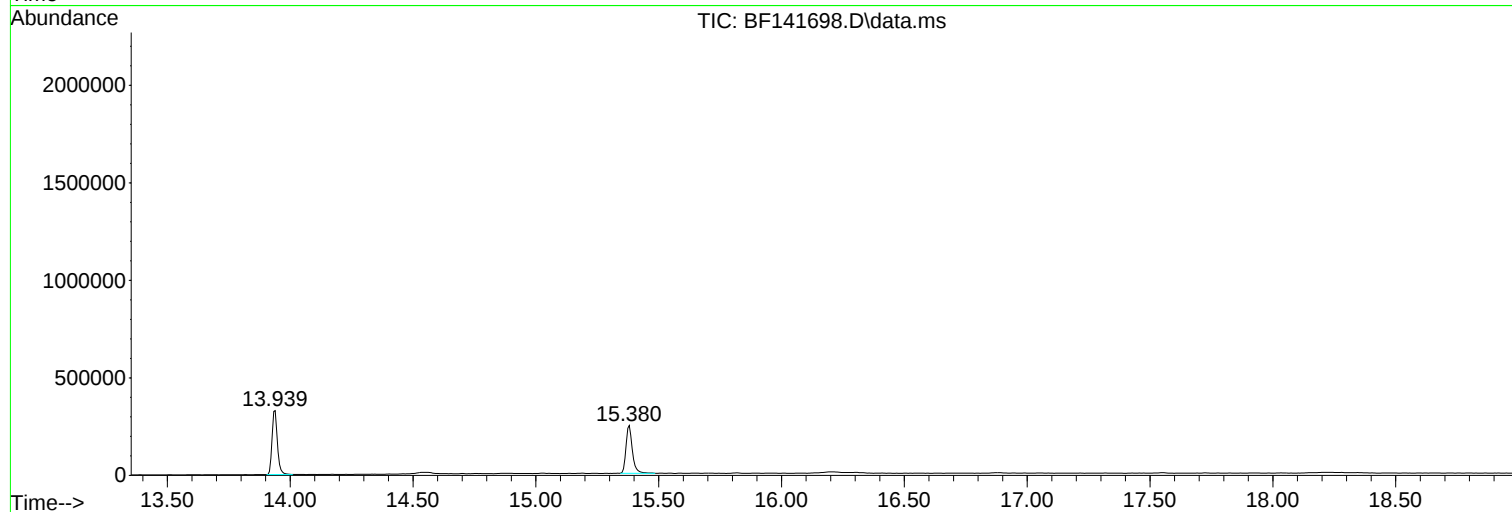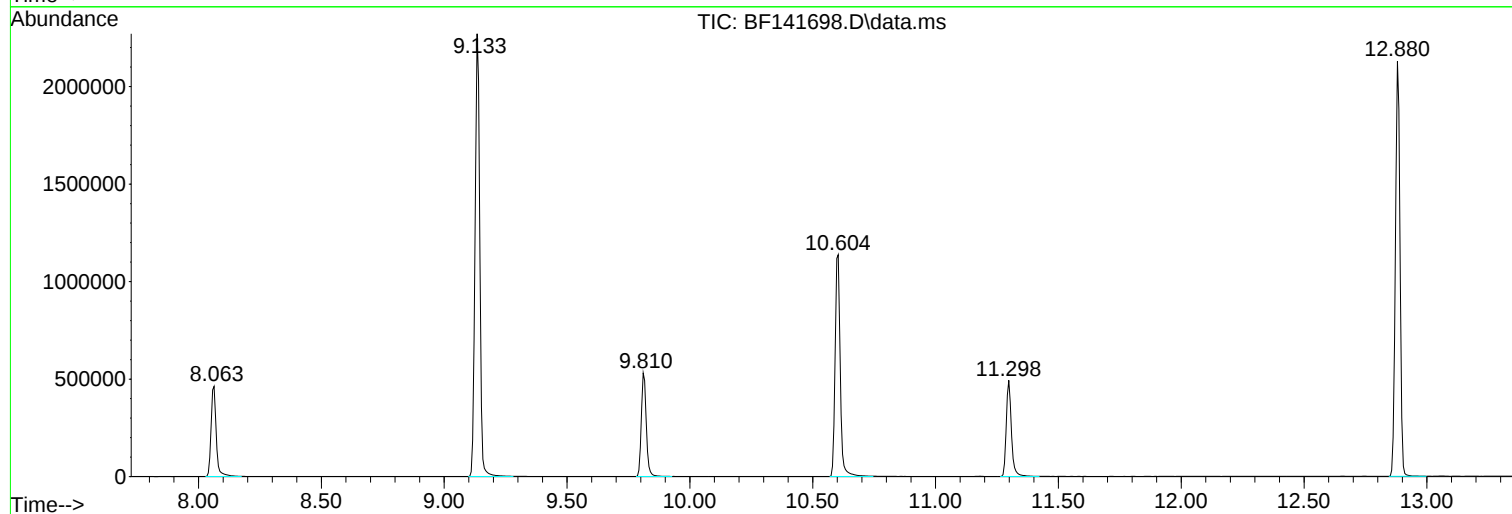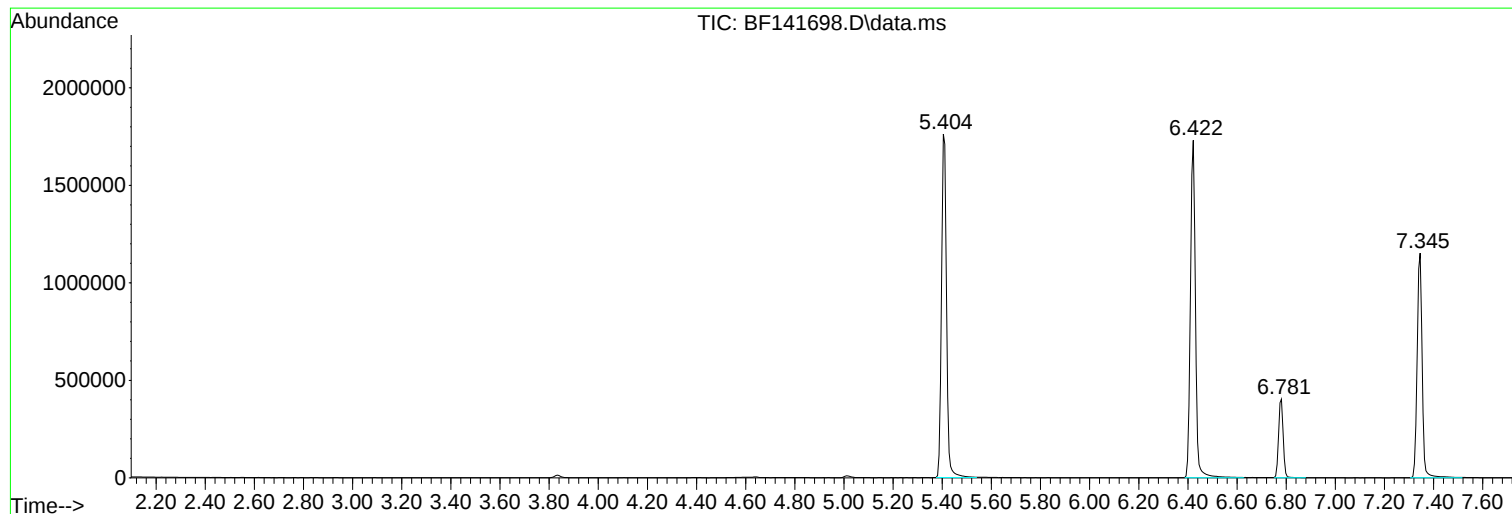

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141698.D
Acq On : 20 Feb 2025 12:33
Operator : RC/JU
Sample : PB166776BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166776BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141698.D
Acq On : 20 Feb 2025 12:33
Operator : RC/JU
Sample : PB166776BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166776BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------