

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF022025\  
 Data File : BF141700.D  
 Acq On : 20 Feb 2025 13:36  
 Operator : RC/JU  
 Sample : Q1383-11  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 OU4-PCS-TC-16-021725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141700.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.399       | 556           | 562         | 582          | rBV      | 1047945        | 1489567       | 82.28%          | 11.950%       |
| 2         | 6.416       | 730           | 735         | 765          | rBV      | 1084486        | 1550444       | 85.64%          | 12.439%       |
| 3         | 6.775       | 791           | 796         | 806          | rBV      | 377997         | 492263        | 27.19%          | 3.949%        |
| 4         | 7.340       | 887           | 892         | 906          | rBV      | 701726         | 975135        | 53.86%          | 7.823%        |
| 5         | 7.610       | 933           | 938         | 952          | rBV      | 12900          | 35684         | 1.97%           | 0.286%        |
| 6         | 8.063       | 1009          | 1015        | 1041         | rBV      | 443714         | 643112        | 35.52%          | 5.160%        |
| 7         | 9.134       | 1191          | 1197        | 1208         | rBV      | 1394992        | 1805679       | 99.74%          | 14.486%       |
| 8         | 9.810       | 1307          | 1312        | 1328         | rBV      | 521033         | 695553        | 38.42%          | 5.580%        |
| 9         | 10.528      | 1429          | 1434        | 1441         | rBV      | 91361          | 124637        | 6.88%           | 1.000%        |
| 10        | 10.598      | 1441          | 1446        | 1464         | rVV      | 735016         | 1035403       | 57.19%          | 8.307%        |
| 11        | 11.298      | 1559          | 1565        | 1585         | rVB      | 494830         | 692120        | 38.23%          | 5.553%        |
| 12        | 11.828      | 1648          | 1655        | 1676         | rBV2     | 83690          | 180722        | 9.98%           | 1.450%        |
| 13        | 12.616      | 1782          | 1789        | 1800         | rBV5     | 12311          | 35127         | 1.94%           | 0.282%        |
| 14        | 12.880      | 1828          | 1834        | 1844         | rBV      | 1415149        | 1810356       | 100.00%         | 14.524%       |
| 15        | 13.933      | 2006          | 2013        | 2023         | rVB      | 360209         | 519564        | 28.70%          | 4.168%        |
| 16        | 15.374      | 2252          | 2258        | 2272         | rVB      | 211676         | 379232        | 20.95%          | 3.042%        |




Sum of corrected areas: 12464598

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF022025\  
Data File : BF141700.D  
Acq On : 20 Feb 2025 13:36  
Operator : RC/JU  
Sample : Q1383-11  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
OU4-PCS-TC-16-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

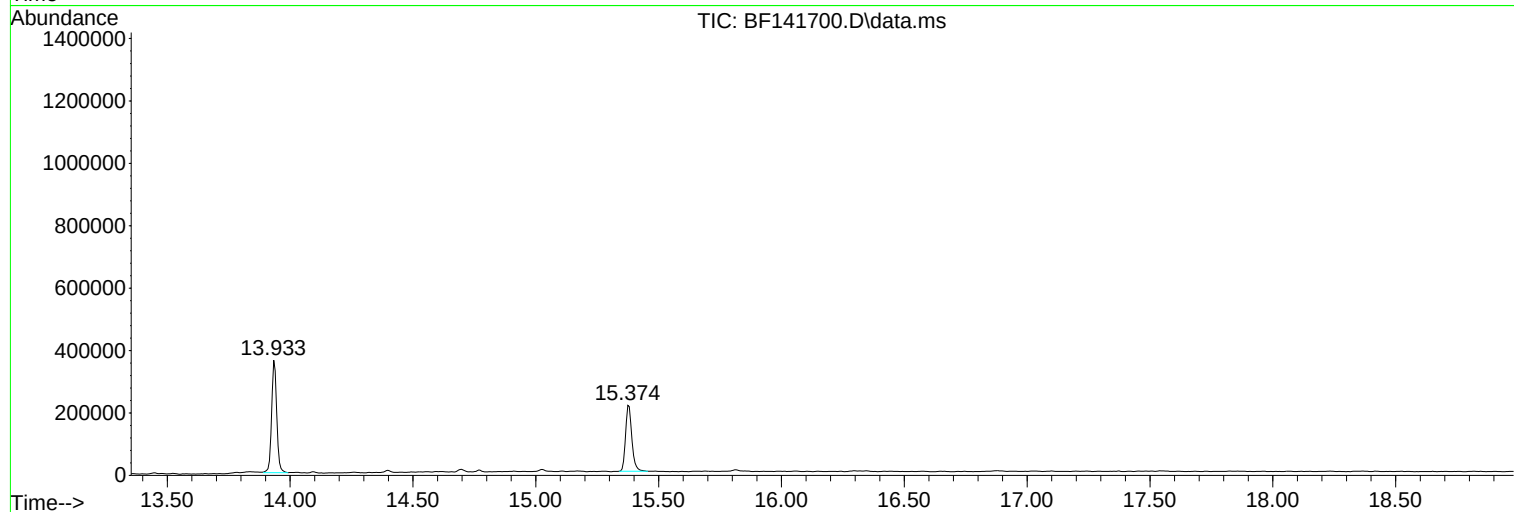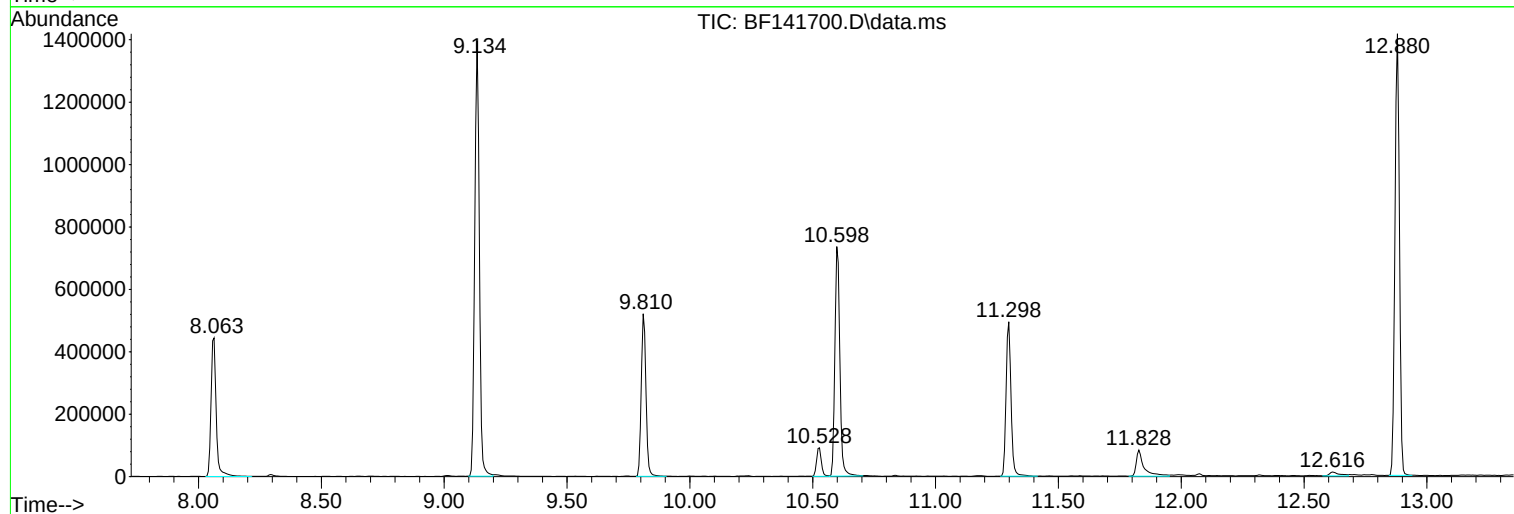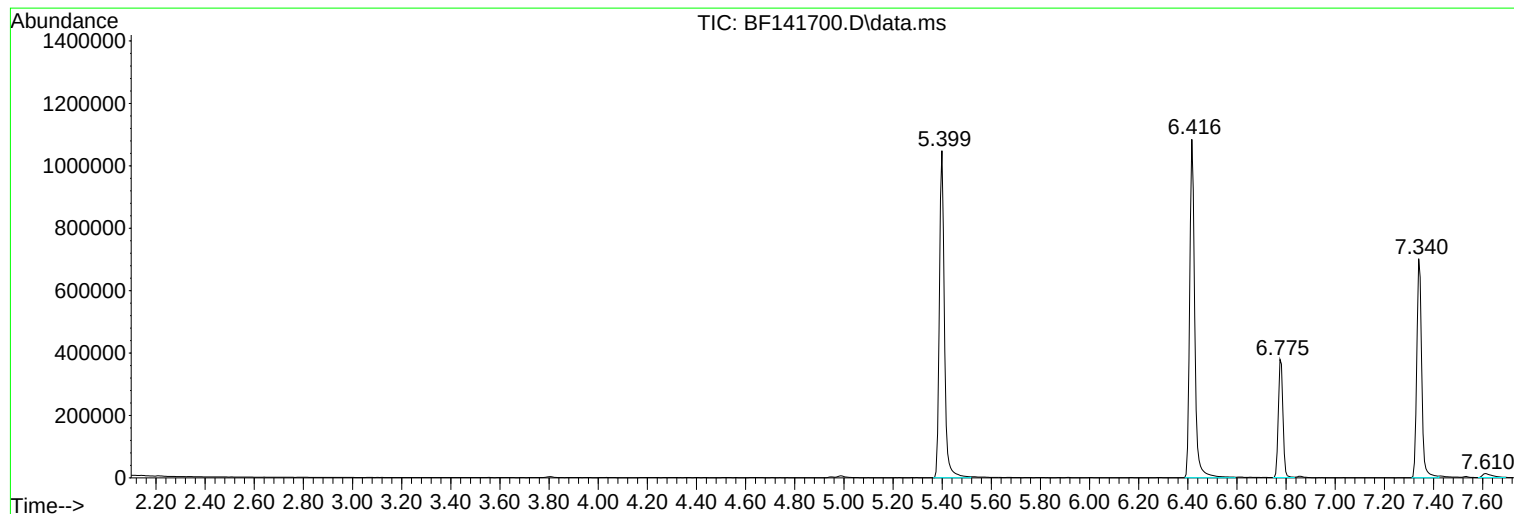

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF022025\  
Data File : BF141700.D  
Acq On : 20 Feb 2025 13:36  
Operator : RC/JU  
Sample : Q1383-11  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
OU4-PCS-TC-16-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF022025\  
Data File : BF141700.D  
Acq On : 20 Feb 2025 13:36  
Operator : RC/JU  
Sample : Q1383-11  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
OU4-PCS-TC-16-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|