

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
 Data File : BF141703.D
 Acq On : 20 Feb 2025 15:07
 Operator : RC/JU
 Sample : Q1383-17
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-TC-19-021725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141703.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.398	557	562	587	rBV	1161300	1620688	80.07%	11.908%
2	6.416	730	735	765	rBV	1188703	1688384	83.41%	12.405%
3	6.781	791	797	806	rBV	403604	532543	26.31%	3.913%
4	7.339	887	892	907	rBV	743976	1073178	53.02%	7.885%
5	7.622	934	940	956	rBV3	12986	41322	2.04%	0.304%
6	8.063	1009	1015	1038	rBV	494339	697823	34.48%	5.127%
7	9.133	1192	1197	1225	rVB	1540468	2024140	100.00%	14.872%
8	9.810	1307	1312	1328	rBV	549682	768202	37.95%	5.644%
9	10.527	1429	1434	1441	rBV	128862	170561	8.43%	1.253%
10	10.604	1441	1447	1464	rVV	791342	1137079	56.18%	8.355%
11	11.298	1560	1565	1585	rVB	555761	768574	37.97%	5.647%
12	11.827	1650	1655	1671	rBV2	46646	101070	4.99%	0.743%
13	12.880	1828	1834	1846	rBV	1526802	1974533	97.55%	14.508%
14	13.827	1984	1995	2007	rBV9	10967	64185	3.17%	0.472%
15	13.939	2008	2014	2027	rVB	345850	518774	25.63%	3.812%
16	15.380	2253	2259	2271	rBV	251796	429198	21.20%	3.153%




Sum of corrected areas: 13610254

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141703.D
Acq On : 20 Feb 2025 15:07
Operator : RC/JU
Sample : Q1383-17
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-19-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

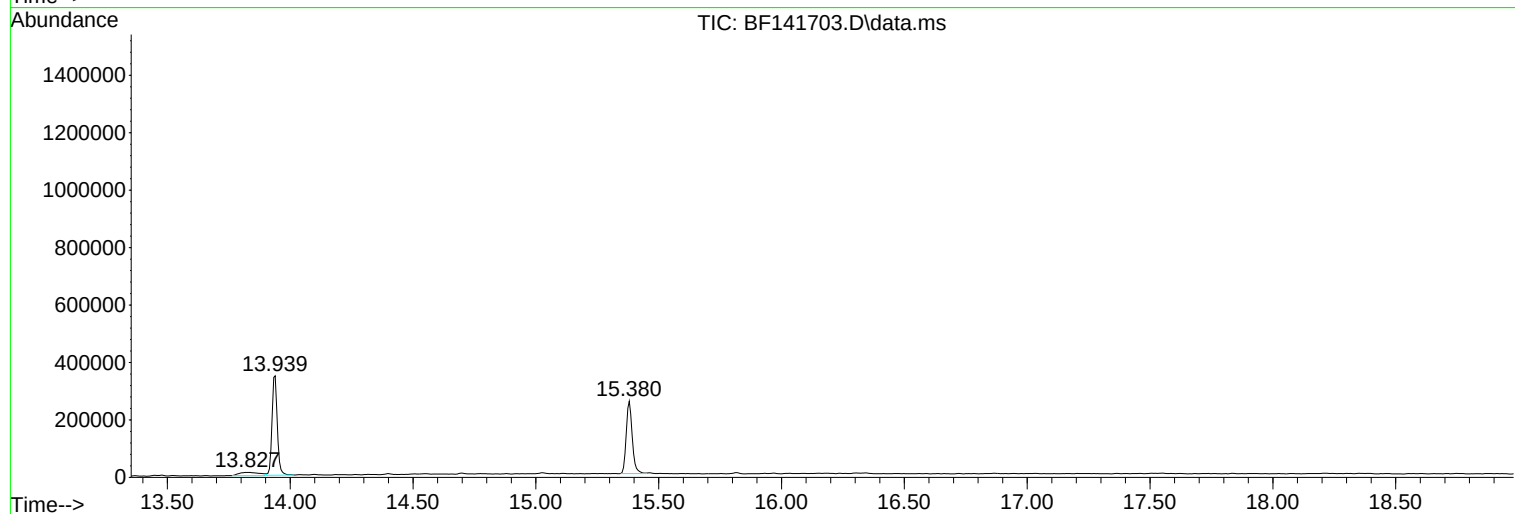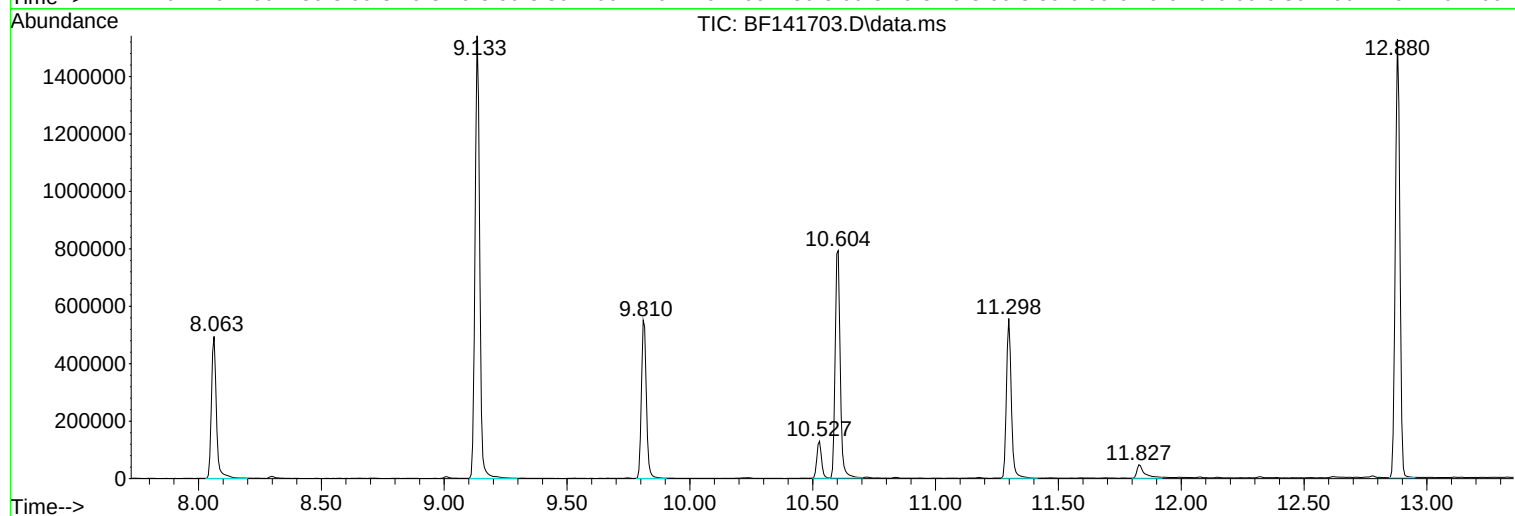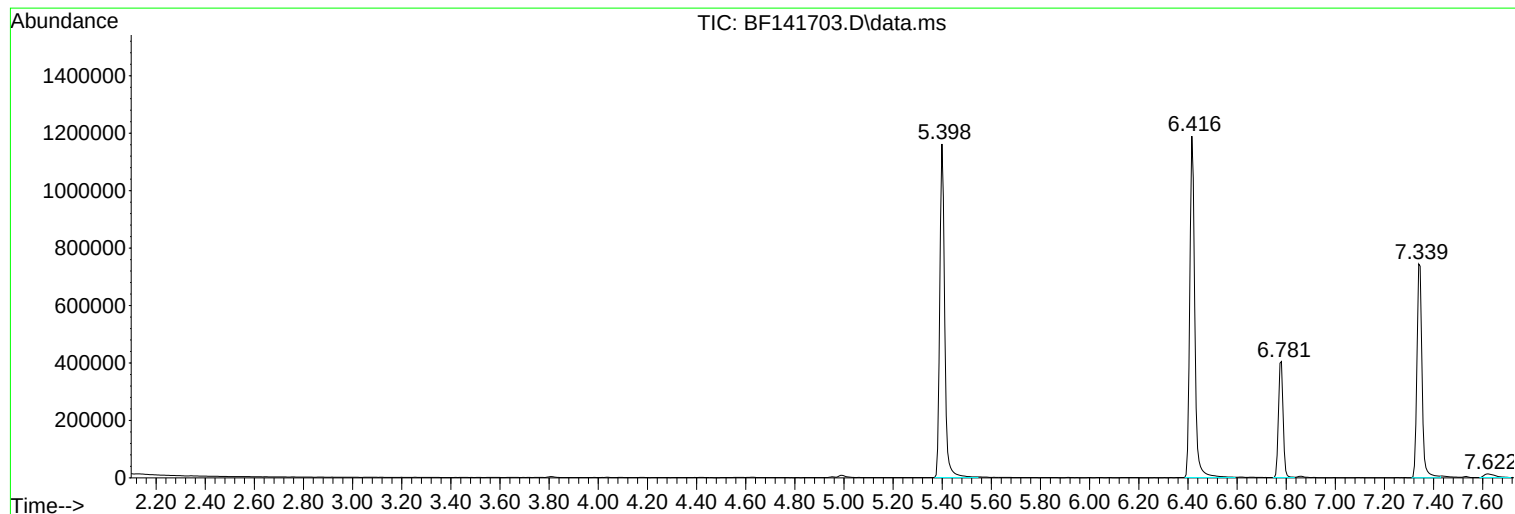

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141703.D
Acq On : 20 Feb 2025 15:07
Operator : RC/JU
Sample : Q1383-17
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-19-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141703.D
Acq On : 20 Feb 2025 15:07
Operator : RC/JU
Sample : Q1383-17
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-19-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------