

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
 Data File : BF141704.D
 Acq On : 20 Feb 2025 15:36
 Operator : RC/JU
 Sample : Q1383-19
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-TC-20-021725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141704.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.398	557	562	580	rBV	1089991	1540765	81.00%	11.884%
2	6.416	730	735	766	rBV	1112911	1580439	83.09%	12.190%
3	6.781	792	797	806	rBV	405342	538965	28.34%	4.157%
4	7.339	887	892	906	rBV	698771	1004877	52.83%	7.750%
5	7.622	934	940	956	rBV3	11277	36541	1.92%	0.282%
6	8.063	1009	1015	1037	rBV	492128	709283	37.29%	5.471%
7	9.133	1191	1197	1209	rBV	1451449	1902111	100.00%	14.671%
8	9.810	1307	1312	1328	rBV	549828	782303	41.13%	6.034%
9	10.527	1429	1434	1441	rBV	117221	157223	8.27%	1.213%
10	10.604	1441	1447	1462	rVV	730173	1044192	54.90%	8.054%
11	11.298	1560	1565	1583	rBV	559038	770162	40.49%	5.940%
12	11.827	1650	1655	1671	rBV2	35771	81764	4.30%	0.631%
13	12.880	1828	1834	1849	rBV	1408804	1800524	94.66%	13.887%
14	13.827	1983	1995	2006	rBV9	11123	60755	3.19%	0.469%
15	13.939	2006	2014	2024	rVB	350347	518470	27.26%	3.999%
16	15.380	2253	2259	2273	rBV	253398	437164	22.98%	3.372%




Sum of corrected areas: 12965538

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141704.D
Acq On : 20 Feb 2025 15:36
Operator : RC/JU
Sample : Q1383-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-20-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

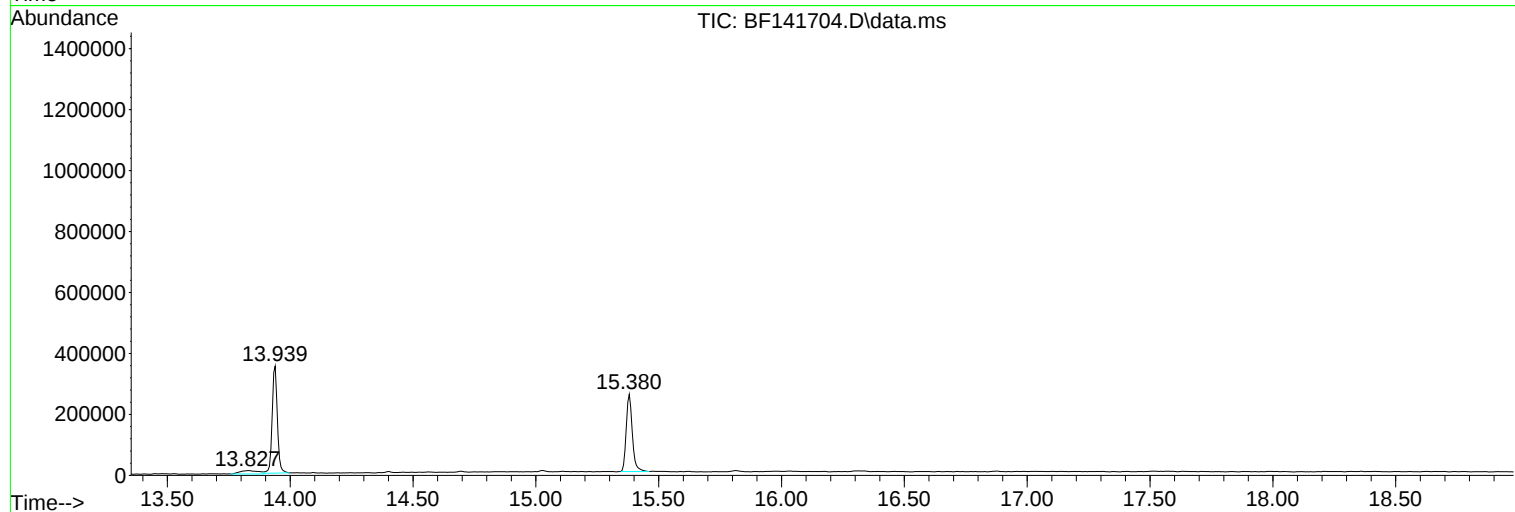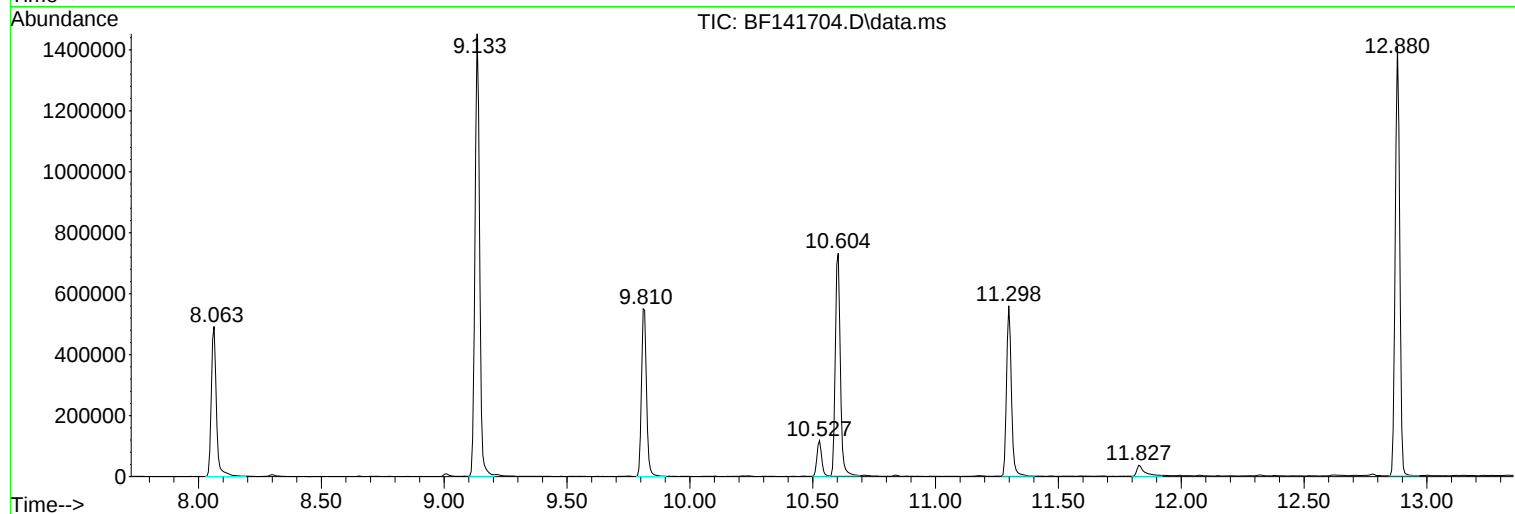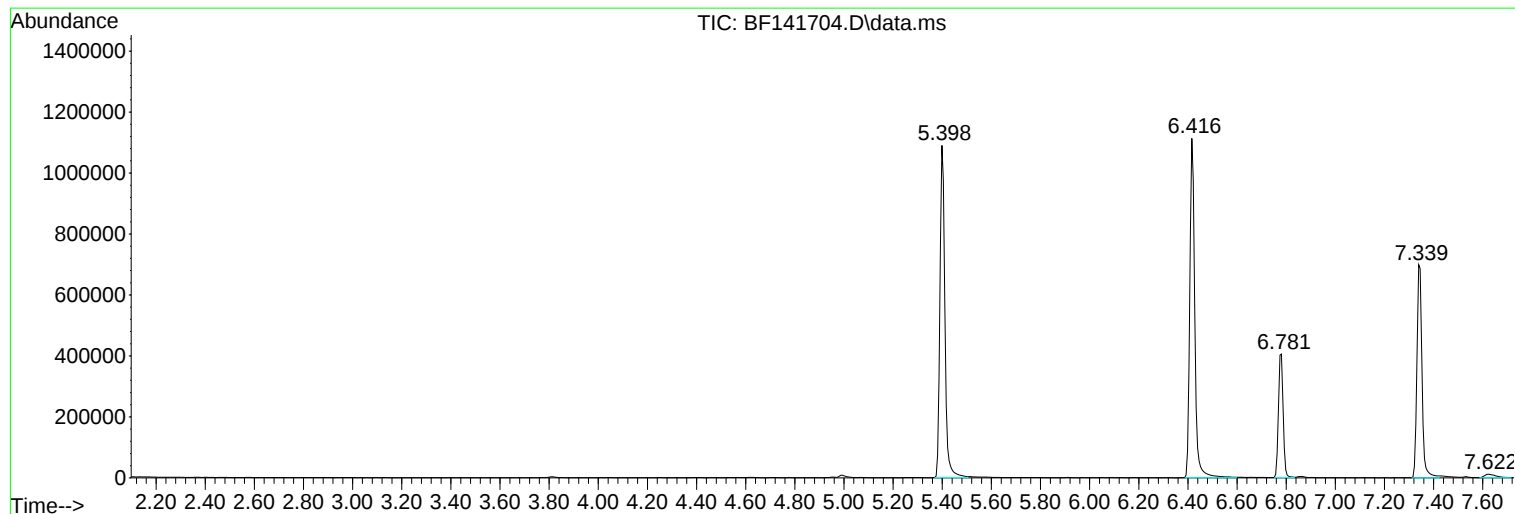

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141704.D
Acq On : 20 Feb 2025 15:36
Operator : RC/JU
Sample : Q1383-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-20-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141704.D
Acq On : 20 Feb 2025 15:36
Operator : RC/JU
Sample : Q1383-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-20-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------