
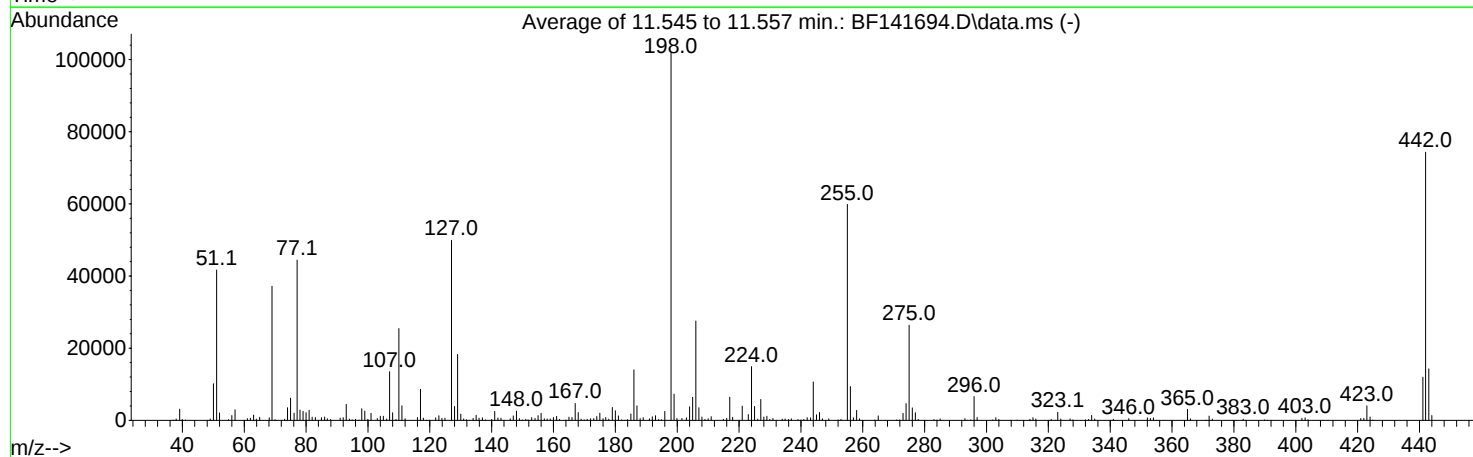


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141694.D
Acq On : 20 Feb 2025 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 06 16:58:59 2025

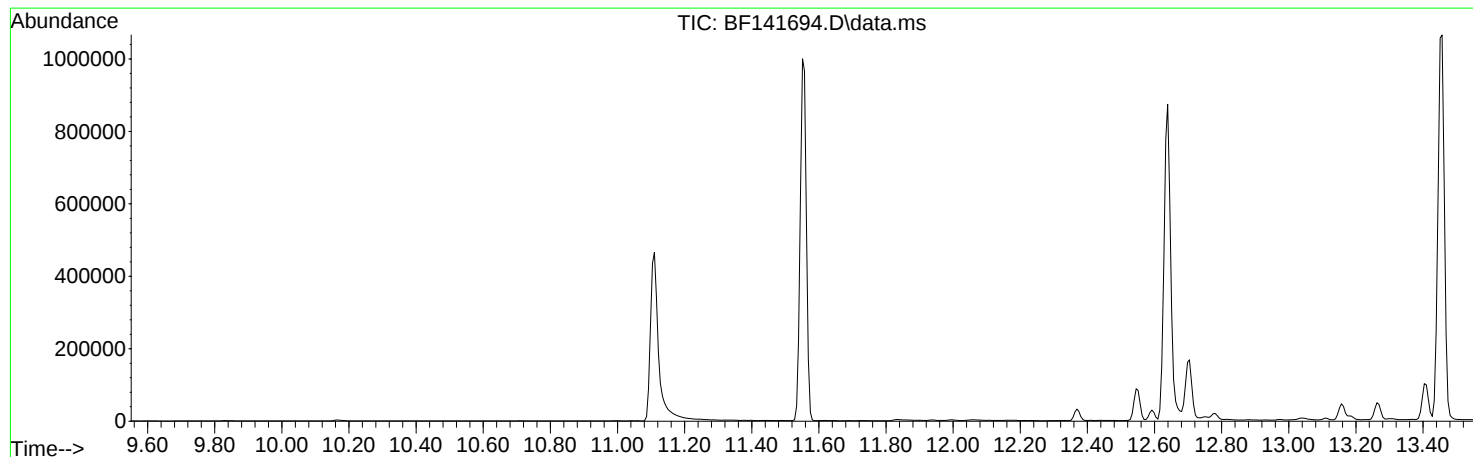

AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.9	41685	PASS
68	69	0.00	2	1.9	697	PASS
69	198	0.00	100	36.4	37160	PASS
70	69	0.00	2	0.6	228	PASS
127	198	10	80	48.9	49901	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	101965	PASS
199	198	5	9	7.1	7260	PASS
275	198	10	60	25.9	26403	PASS
365	198	1	100	3.0	3061	PASS
441	198	0.01	100	11.8	11986	PASS
442	442	50	100	100.0	74336	PASS
443	442	15	24	19.2	14264	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/20/2025	BNA_F	<u>BF141694.D</u>
Compound Name	Response	Retention Time
DDT	283316	13.457
DDD	15994	13.157
DDE	440	12.822
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16434	299750	5.48

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141694.D
Acq On : 20 Feb 2025 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 20 11:48:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

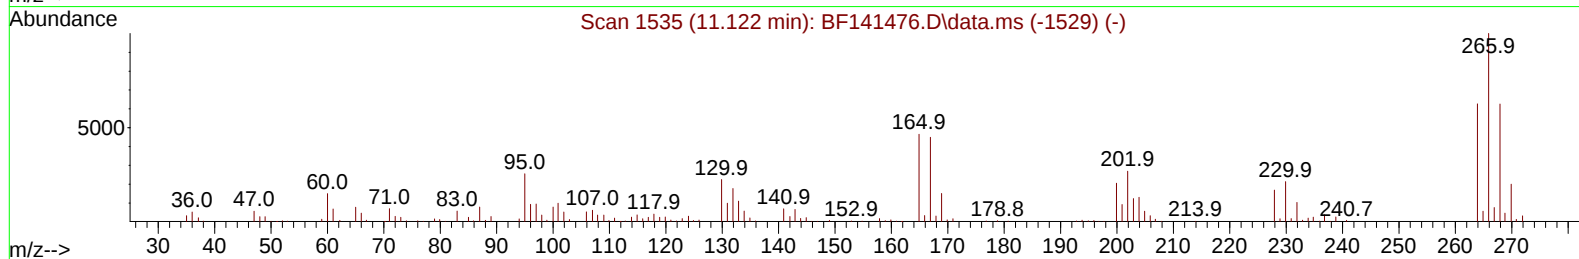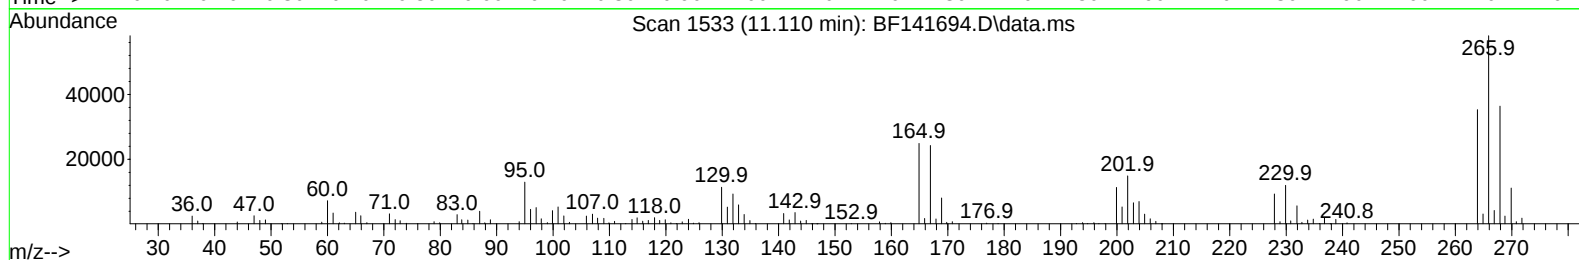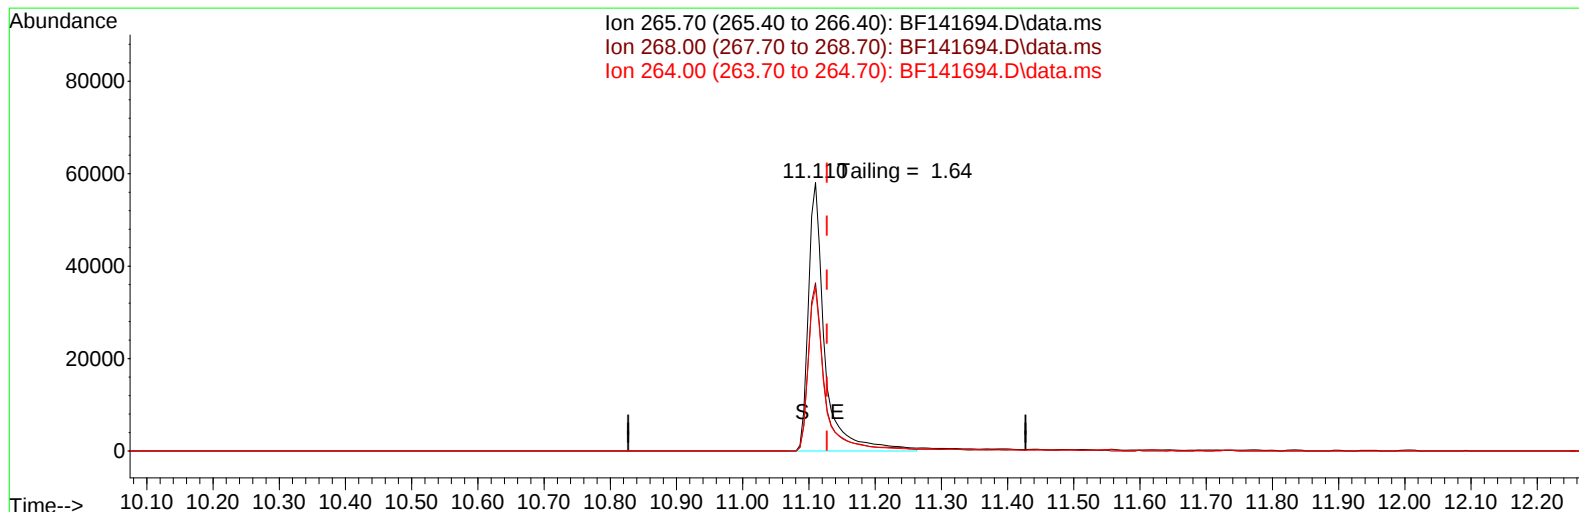

TIC: BF141694.D\data.ms

(70) Pentachlorophenol (C)

11.110min (-0.017) 22081.71 ng




response 100097

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.69
264.00	62.60	60.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141694.D
Acq On : 20 Feb 2025 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 20 11:48:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

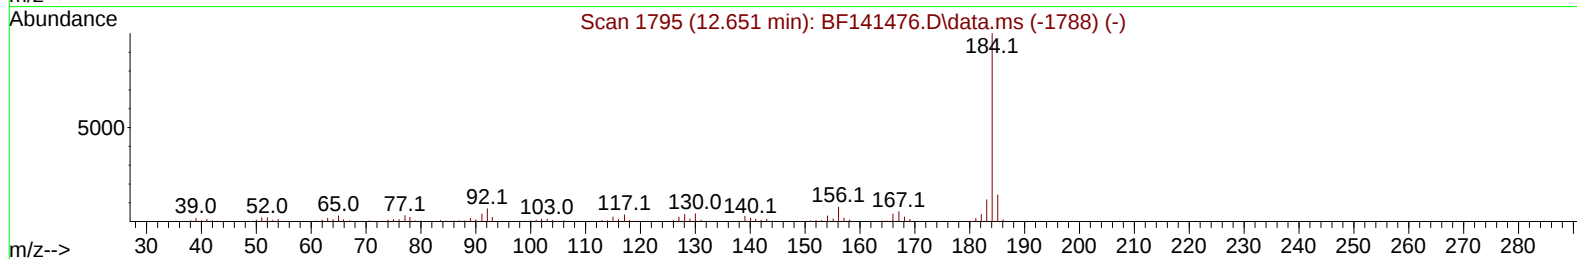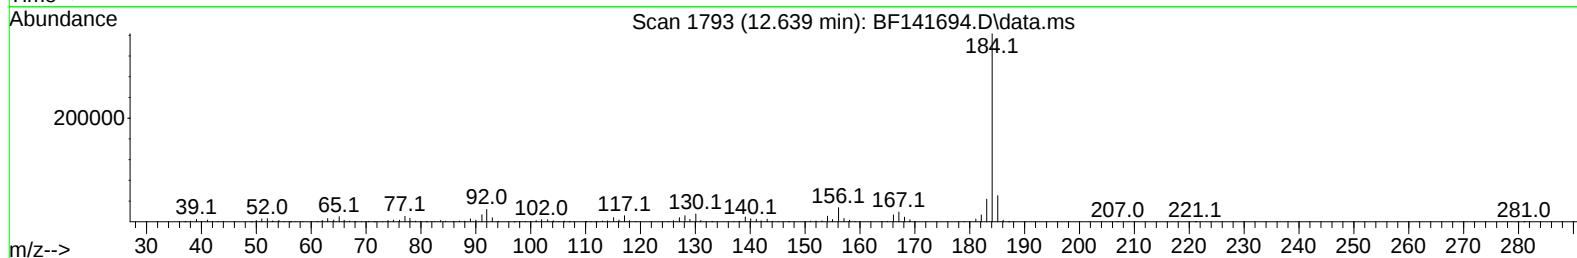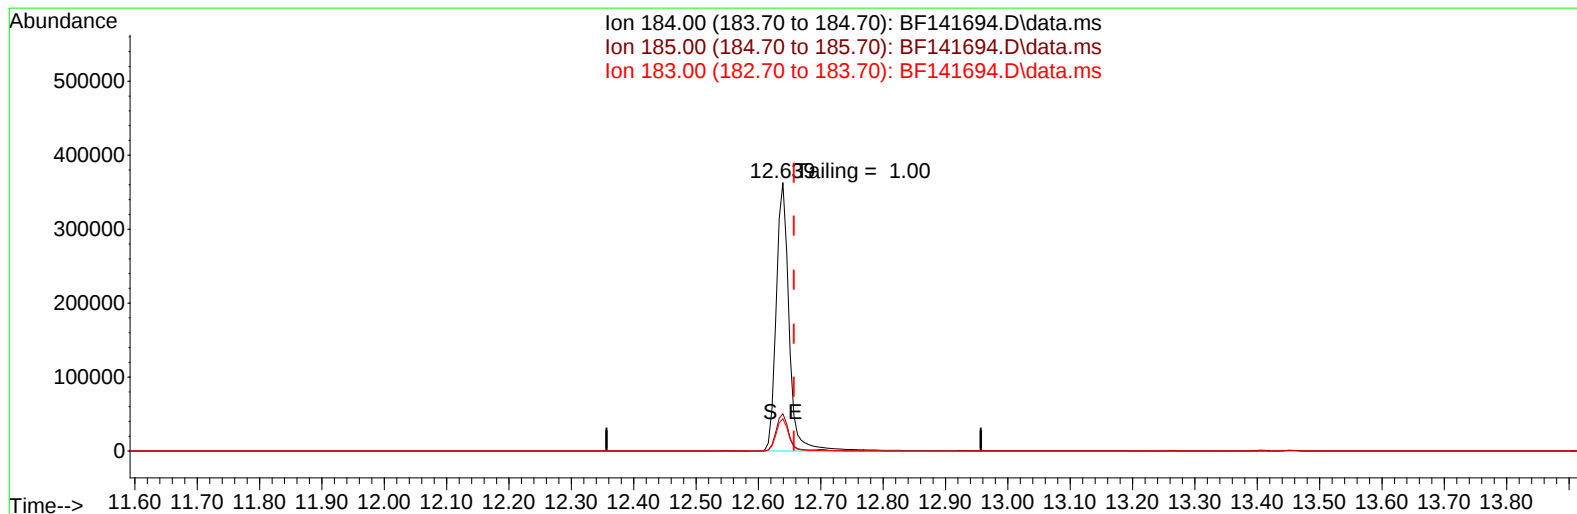

TIC: BF141694.D\data.ms

(77) Benzidine

12.639min (-0.017) 0.00 ng

response 526516

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.88
183.00	11.60	12.04
0.00	0.00	0.00