

Data Path : Z:\HPCHEM1\BNA F\DATA\BF022118\
 Data File : BF103135.D
 Acq On : 21 Feb 2018 14:44
 Operator : SJ/JU
 Sample : J1622-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Feb 21 15:21:12 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 16 14:34:49 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.88	152	169540	20.00	ng	0.00
21) Naphthalene-d8	8.16	136	703368	20.00	ng	0.00
38) Acenaphthene-d10	9.92	164	276583	20.00	ng	0.00
63) Phenanthrene-d10	11.40	188	418272	20.00	ng	0.00
75) Chrysene-d12	14.05	240	342128	20.00	ng	0.00
86) Perylene-d12	15.54	264	298233	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.51	112	1287883	115.36	ng	0.02
7) Phenol-d6	6.52	99	1520046	113.08	ng	0.00
23) Nitrobenzene-d5	7.45	82	968766	95.55	ng	0.00
41) 2,4,6-Tribromophenol	10.71	330	252718	113.52	ng	0.00
44) 2-Fluorobiphenyl	9.23	172	1381093	82.86	ng	0.00
78) Terphenyl-d14	12.99	244	958575	66.34	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.45	70	129179	14.576	ng	# 79
25) Isophorone	7.45	82	968751	41.493	ng	# 64
47) 2-Nitroaniline	9.33	65	230	3.510	ng	# 2
49) Dimethylphthalate	9.63	163	68150	3.160	ng	# 98
50) 2,6-Dinitrotoluene	9.92	165	35996	8.773	ng	# 26
56) 2,4-Dinitrotoluene	9.92	165	35996	9.198	ng	# 24
64) 4,6-Dinitro-2-methylphenol	10.71	198	434	9.023	ng	# 1
66) 4-Bromophenyl-phenylether	10.71	248	16699	3.774	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF022118\
Data File : BF103135.D
Acq On : 21 Feb 2018 14:44
Operator : SJ/JU
Sample : J1622-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Feb 21 15:21:12 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 16 14:34:49 2018
Response via : Initial Calibration

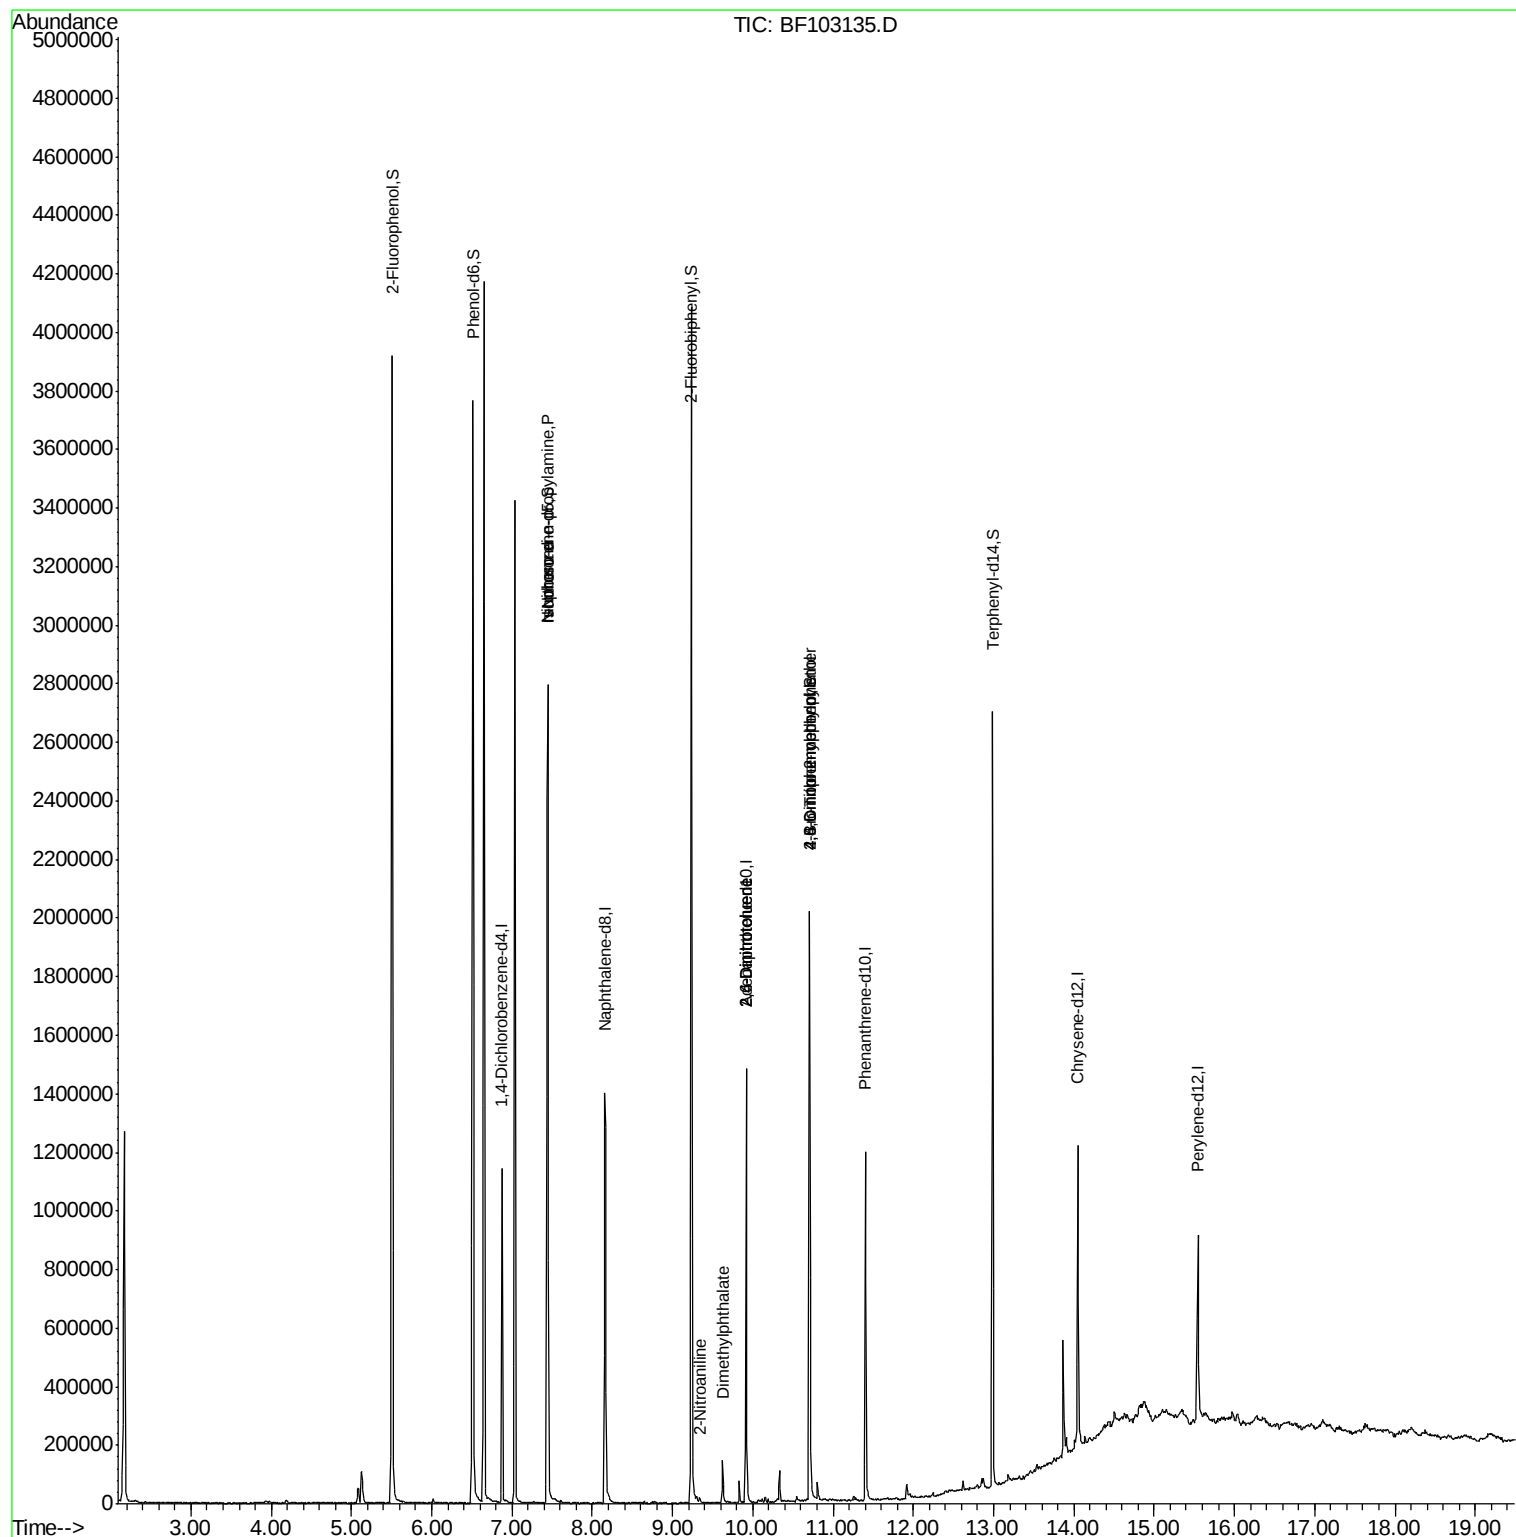

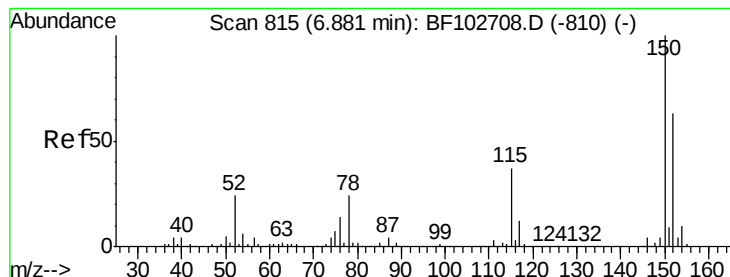


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.88 min Scan# 815
Delta R.T. -0.00 min
Lab File: BF103135.D
Acq: 21 Feb 2018 14:44

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	156.2	124.6	186.8
115	60.2	50.1	75.1

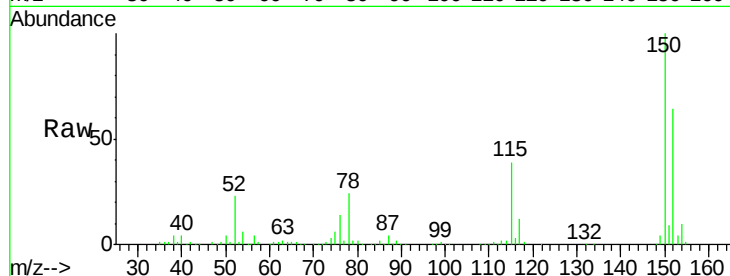


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

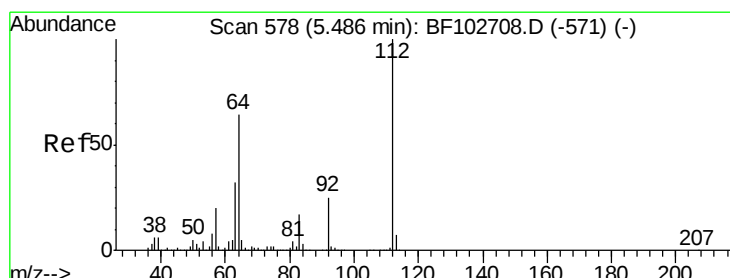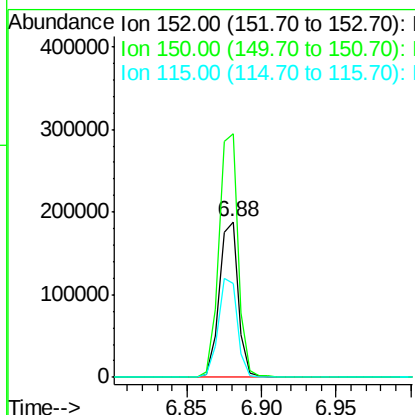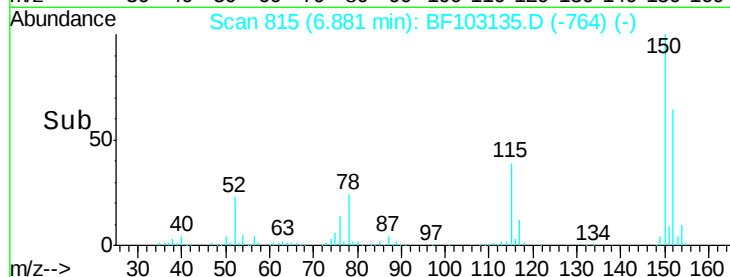



#5



2-Fluorophenol
Concen: 115.363 ng
RT: 5.51 min Scan# 582
Delta R.T. 0.02 min
Lab File: BF103135.D
Acq: 21 Feb 2018 14:44

Tgt Ion	Ratio	Lower	Upper
112	100		
64	62.5	47.9	71.9
63	32.0	23.7	35.5

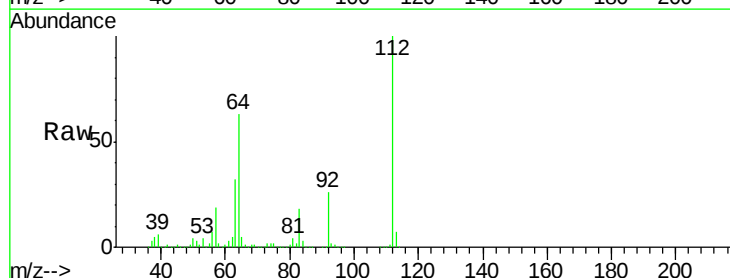

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

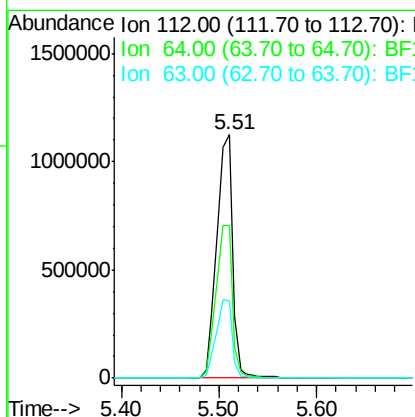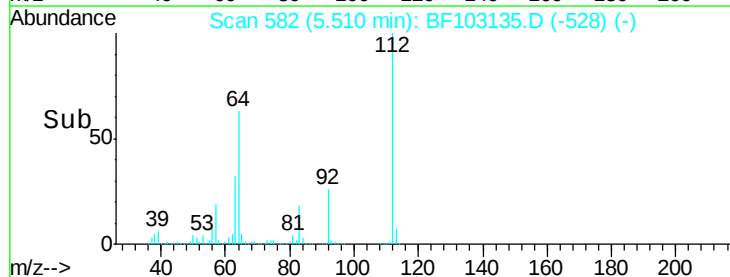

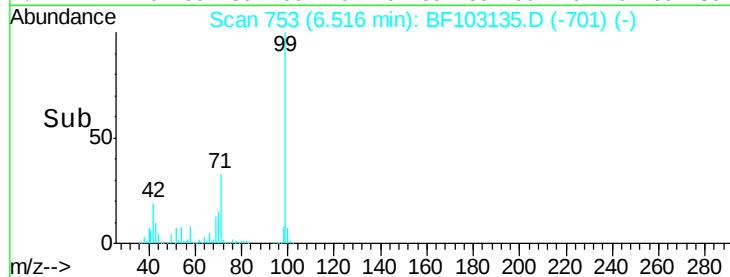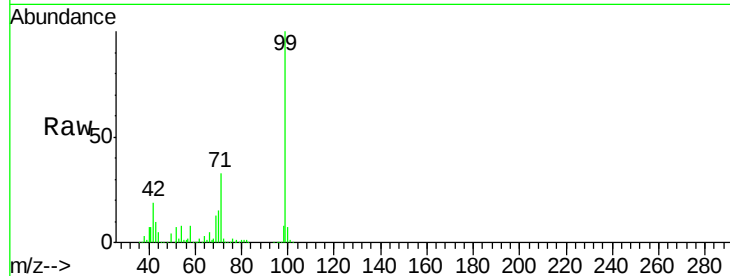

#7

Phenol-d6

Concen: 113.083 ng

RT: 6.52 min Scan# 753





Delta R.T. 0.01 min

Lab File: BF103135.D

Acq: 21 Feb 2018 14:44

Tot Ion: 99 Resp: 1520046

Ion	Ratio	Lower	Upper
99	100		
42	18.5	14.5	21.7
71	32.8	25.4	38.0

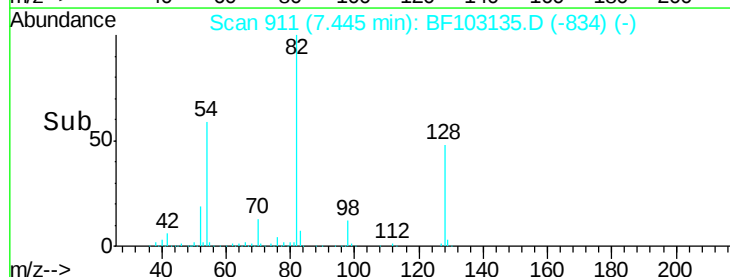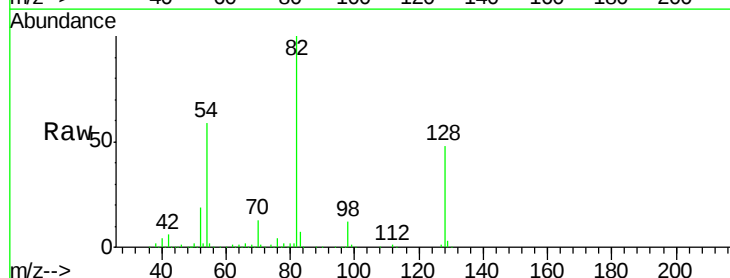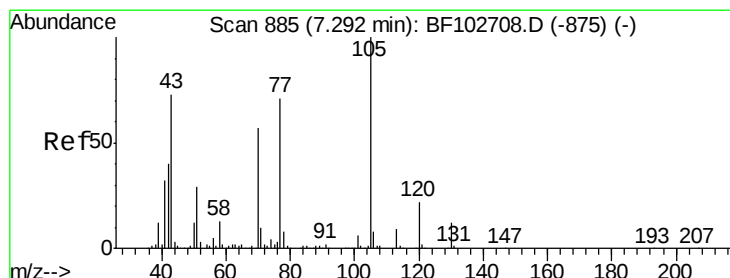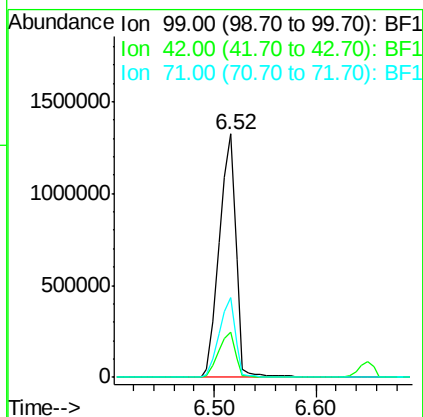

#19

n-Nitroso-di-n-propylamine

Concen: 14.576 ng

RT: 7.45 min Scan# 911


Delta R.T. 0.15 min

Lab File: BF103135.D

Acq: 21 Feb 2018 14:44

Tgt Ion: 70 Resp: 129179

Ion	Ratio	Lower	Upper
70	100		
42	48.8	47.5	71.3
101	0.0	7.4	11.2#
130	2.3	16.6	25.0#

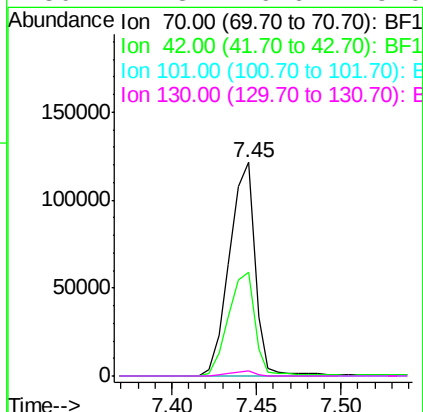



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.16 min Scan# 1032

Delta R.T. -0.01 min

Lab File: BF103135.D

Acq: 21 Feb 2018 14:44

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 703368


Ion Ratio Lower Upper

136 100

137 11.1 8.9 13.3

54 9.9 6.6 9.8#

68 6.9 5.0 7.4






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

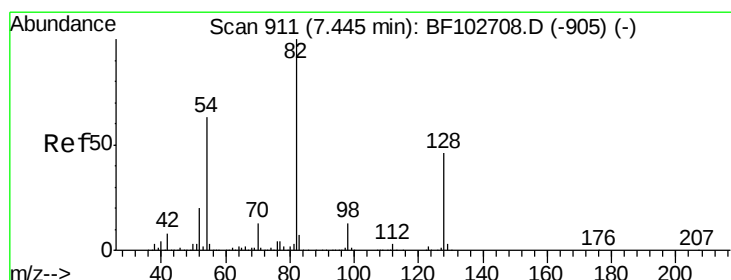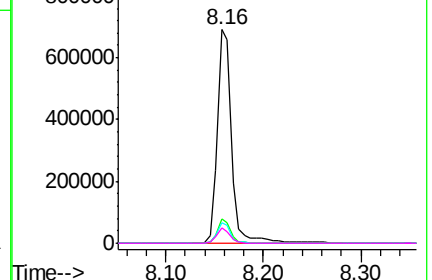

#23

Nitrobenzene-d5

Concen: 95.546 ng

RT: 7.45 min Scan# 911

Delta R.T. -0.00 min

Lab File: BF103135.D

Acq: 21 Feb 2018 14:44


Tgt Ion: 82 Resp: 968766

Ion Ratio Lower Upper

82 100

128 48.2 36.1 54.1



54 58.8 41.4 62.2




Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

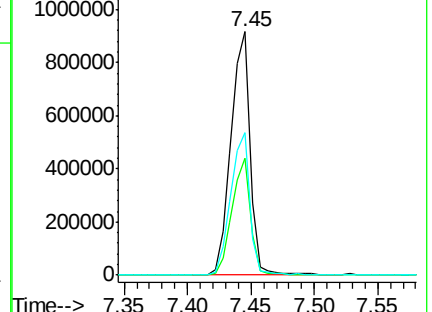

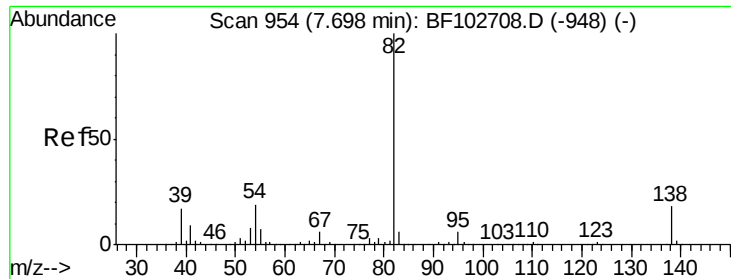

#25

Isophorone

Concen: 41.493 ng

RT: 7.45 min Scan# 911

Delta R.T. -0.25 min

Lab File: BF103135.D

Acq: 21 Feb 2018 14:44

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 968751

Ion Ratio Lower Upper




82 100

95 0.0 5.2 7.8#

138 0.0 14.9 22.3#

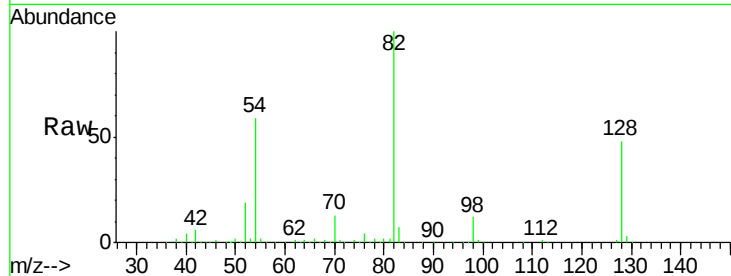

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1

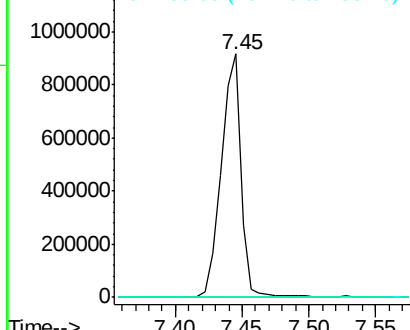

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.92 min Scan# 1331

Delta R.T. -0.01 min

Lab File: BF103135.D

Acq: 21 Feb 2018 14:44


Tgt Ion: 164 Resp: 276583

Ion Ratio Lower Upper



164 100


162 104.6 86.1 129.1

160 45.6 38.3 57.5



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E




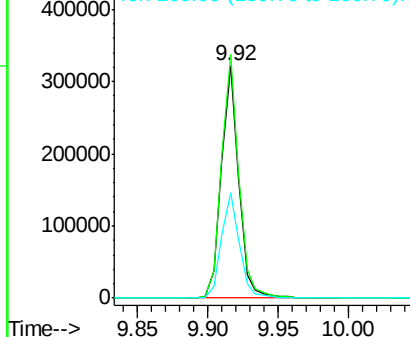




#41
 2,4,6-Tribromophenol
 Concen: 113.521 ng
 RT: 10.71 min Scan# 1466
 Delta R.T. -0.00 min
 Lab File: BF103135.D
 Acq: 21 Feb 2018 14:44




Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	102.5	77.0	115.6
141	39.3	29.9	44.9

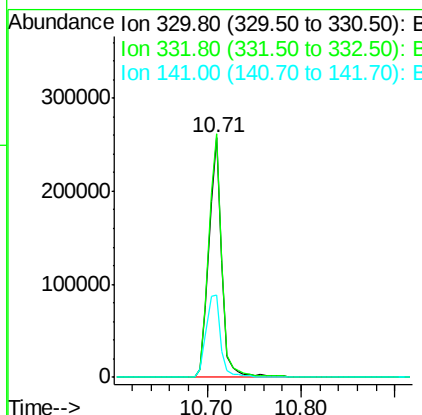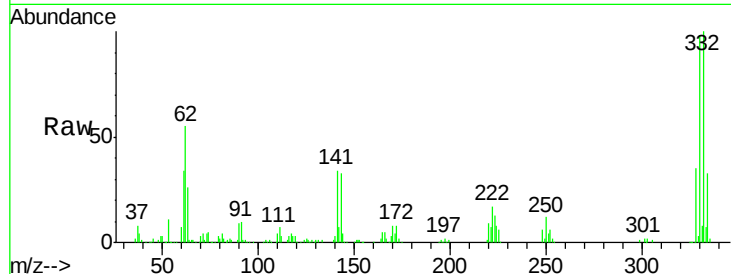

#44
 2-Fluorobiphenyl
 Concen: 82.858 ng
 RT: 9.23 min Scan# 1215
 Delta R.T. -0.01 min
 Lab File: BF103135.D
 Acq: 21 Feb 2018 14:44

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.7	29.7	44.5
170	24.5	19.6	29.4

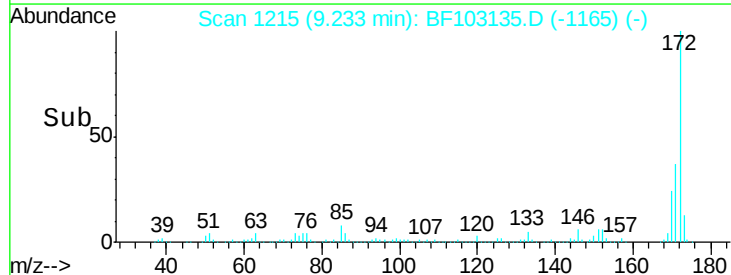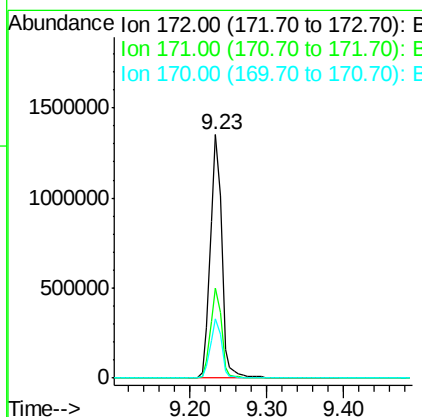



#47

2-Nitroaniline

Concen: 3.510 ng

RT: 9.33 min Scan# 1232

Delta R.T. -0.13 min

Lab File: BF103135.D

Acq: 21 Feb 2018 14:44

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 65 Resp: 230

Ion Ratio Lower Upper

65 100

92 0.0 55.8 83.6#

138 0.0 91.2 136.8#



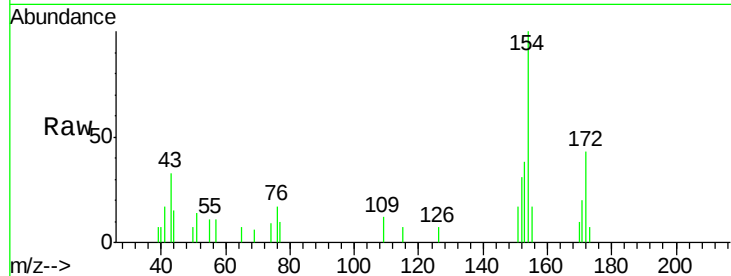


Abundance Ion 65.00 (64.70 to 65.70): BF1

Ion 92.00 (91.70 to 92.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

Time-->

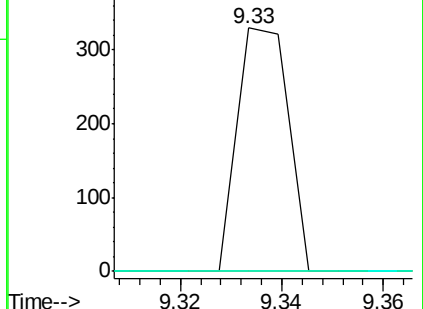

#49

Dimethylphthalate

Concen: 3.160 ng

RT: 9.63 min Scan# 1282

Delta R.T. -0.01 min

Lab File: BF103135.D

Acq: 21 Feb 2018 14:44


Tgt Ion: 163 Resp: 68150

Ion Ratio Lower Upper

163 100

194 3.8 2.7 4.1

164 9.5 8.2 12.2






Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

Time-->



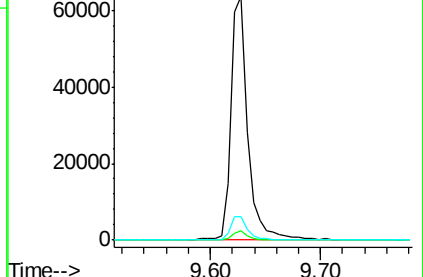





#50
 2,6-Dinitrotoluene
 Concen: 8.773 ng
 RT: 9.92 min Scan# 1331
 Delta R.T. 0.21 min
 Lab File: BF103135.D
 Acq: 21 Feb 2018 14:44




Instrument :
 BNA_F
 ClientSampled :


Tot Ion	Ratio	Lower	Upper
165	100		
63	1.9	44.7	67.1#
89	1.6	44.0	66.0#

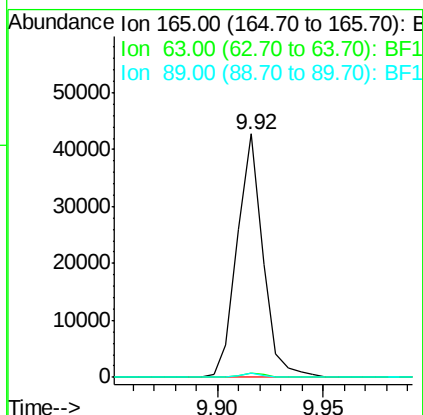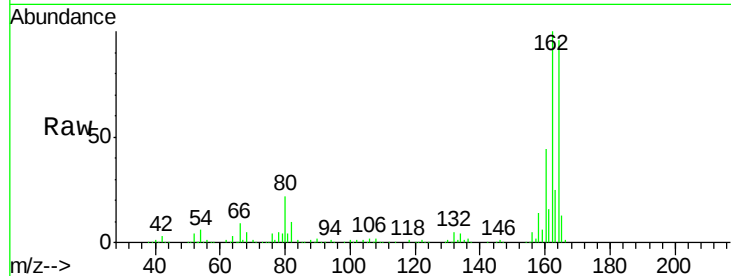

#56
 2,4-Dinitrotoluene
 Concen: 9.198 ng
 RT: 9.92 min Scan# 1331
 Delta R.T. -0.19 min
 Lab File: BF103135.D
 Acq: 21 Feb 2018 14:44

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.9	36.4	54.6#
89	1.6	57.8	86.6#
182	0.0	1.6	2.4#



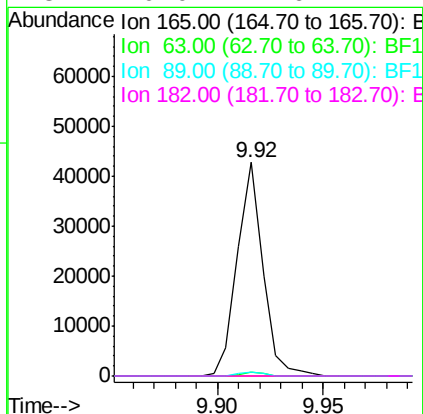
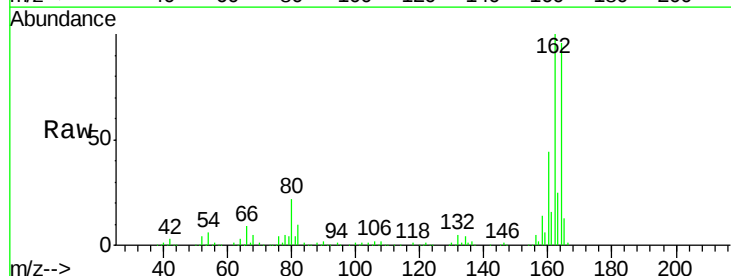


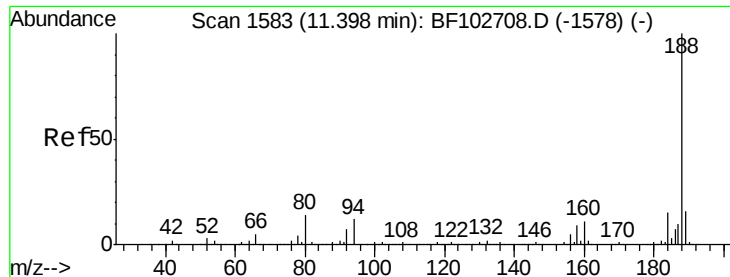

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.40 min Scan# 1584
Delta R.T. -0.01 min
Lab File: BF103135.D
Acq: 21 Feb 2018 14:44




Instrument :
BNA_F
ClientSampleId :


Tot Ion:188 Resp: 418272
Ion Ratio Lower Upper
188 100
94 11.3 8.5 12.7
80 12.3 9.2 13.8

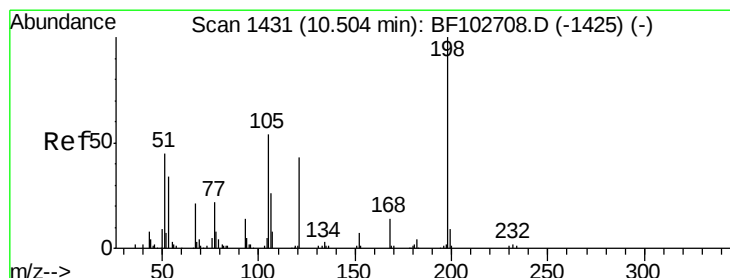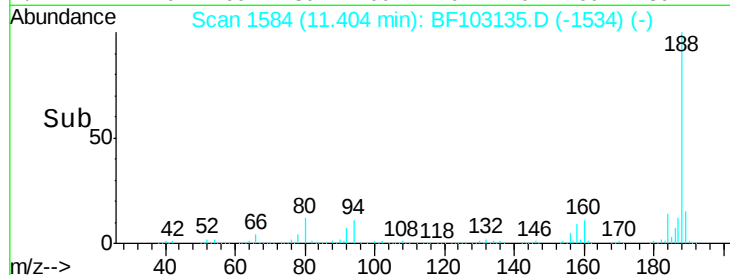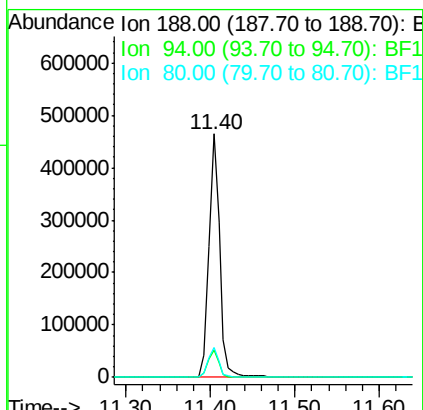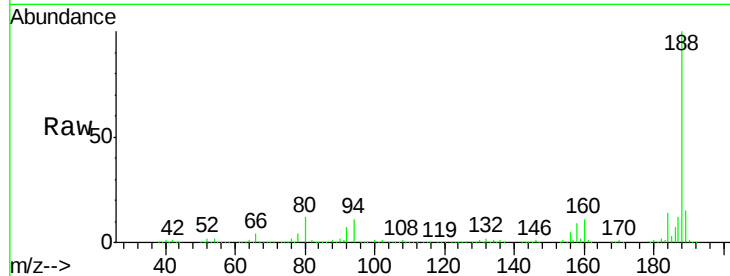

#64
4,6-Dinitro-2-methylphenol
Concen: 9.023 ng
RT: 10.71 min Scan# 1466
Delta R.T. 0.19 min
Lab File: BF103135.D
Acq: 21 Feb 2018 14:44

Tgt Ion:198 Resp: 434
Ion Ratio Lower Upper
198 100
51 206.7 37.7 77.7#
105 194.1 36.3 76.3#

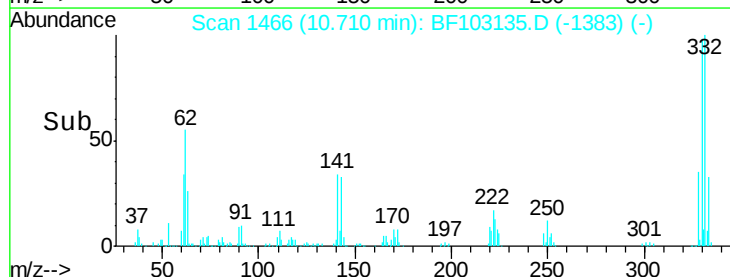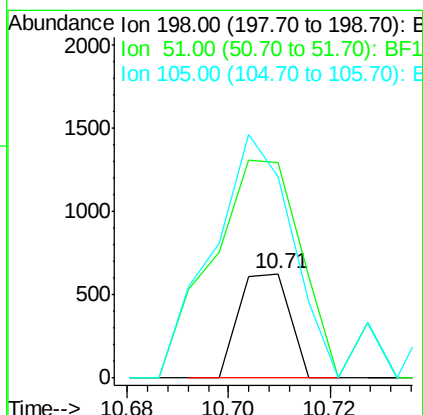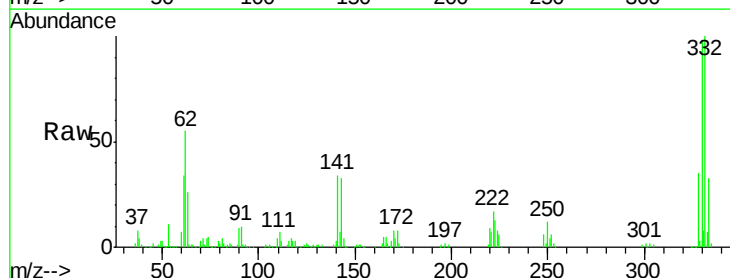


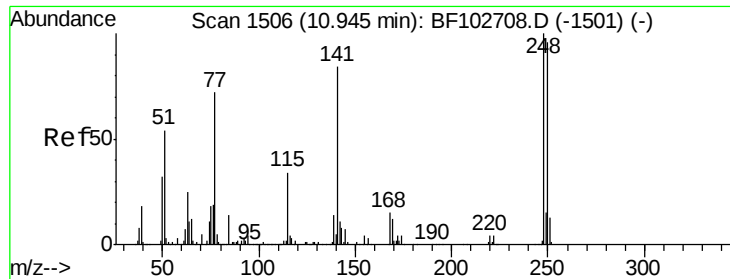




#66
 4-Bromophenyl-phenylether
 Concen: 3.774 ng
 RT: 10.71 min Scan# 1466
 Delta R.T. -0.24 min
 Lab File: BF103135.D
 Acq: 21 Feb 2018 14:44

Instrument :
 BNA_F
 ClientSampled :

Tot Ion:248 Resp: 16699
 Ion Ratio Lower Upper
 248 100
 250 200.5 76.9 115.3#
 141 546.4 74.4 111.6#

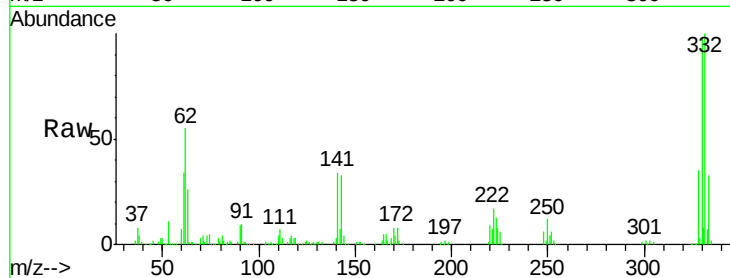


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

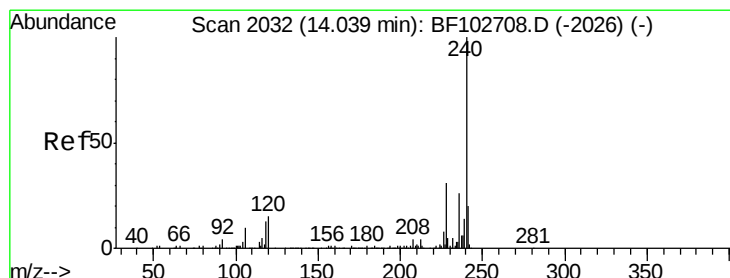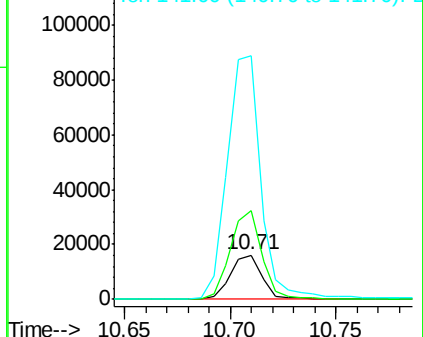
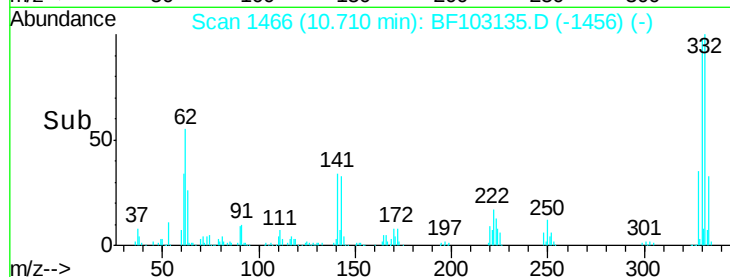



#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 14.05 min Scan# 2034
 Delta R.T. -0.01 min
 Lab File: BF103135.D
 Acq: 21 Feb 2018 14:44

Tgt Ion:240 Resp: 342128
 Ion Ratio Lower Upper
 240 100
 120 15.3 9.5 14.3#
 236 27.7 20.7 31.1

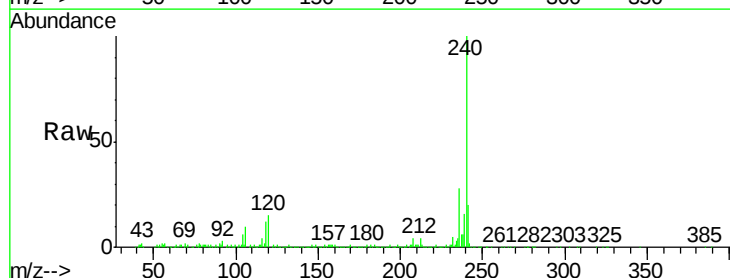

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E



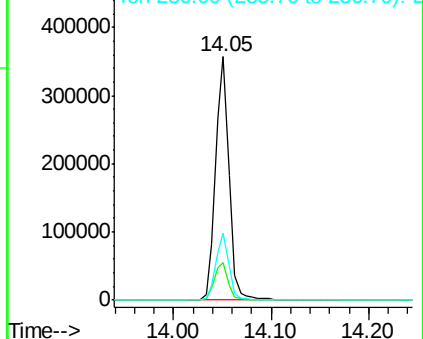
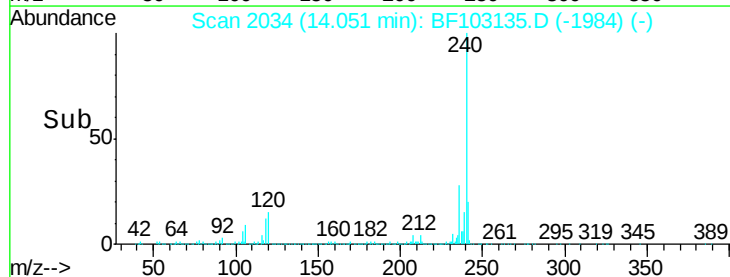




#78
 Terphenyl-d14
 Concen: 66.340 ng
 RT: 12.99 min Scan# 1854
 Delta R.T. -0.00 min
 Lab File: BF103135.D
 Acq: 21 Feb 2018 14:44

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:244 Resp: 958575
 Ion Ratio Lower Upper
 244 100
 212 6.8 5.4 8.0
 122 13.4 11.0 16.4

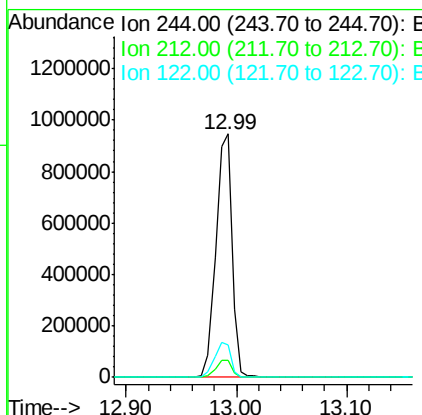

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.54 min Scan# 2288
 Delta R.T. -0.00 min
 Lab File: BF103135.D
 Acq: 21 Feb 2018 14:44

Tgt Ion:264 Resp: 298233
 Ion Ratio Lower Upper
 264 100
 260 24.4 19.2 28.8
 265 21.5 17.5 26.3

