


Data Path : Z:\HPCHEM1\BNA F\DATA\BF022118\
 Data File : BF103126.D
 Acq On : 21 Feb 2018 10:37
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 16 14:34:49 2018

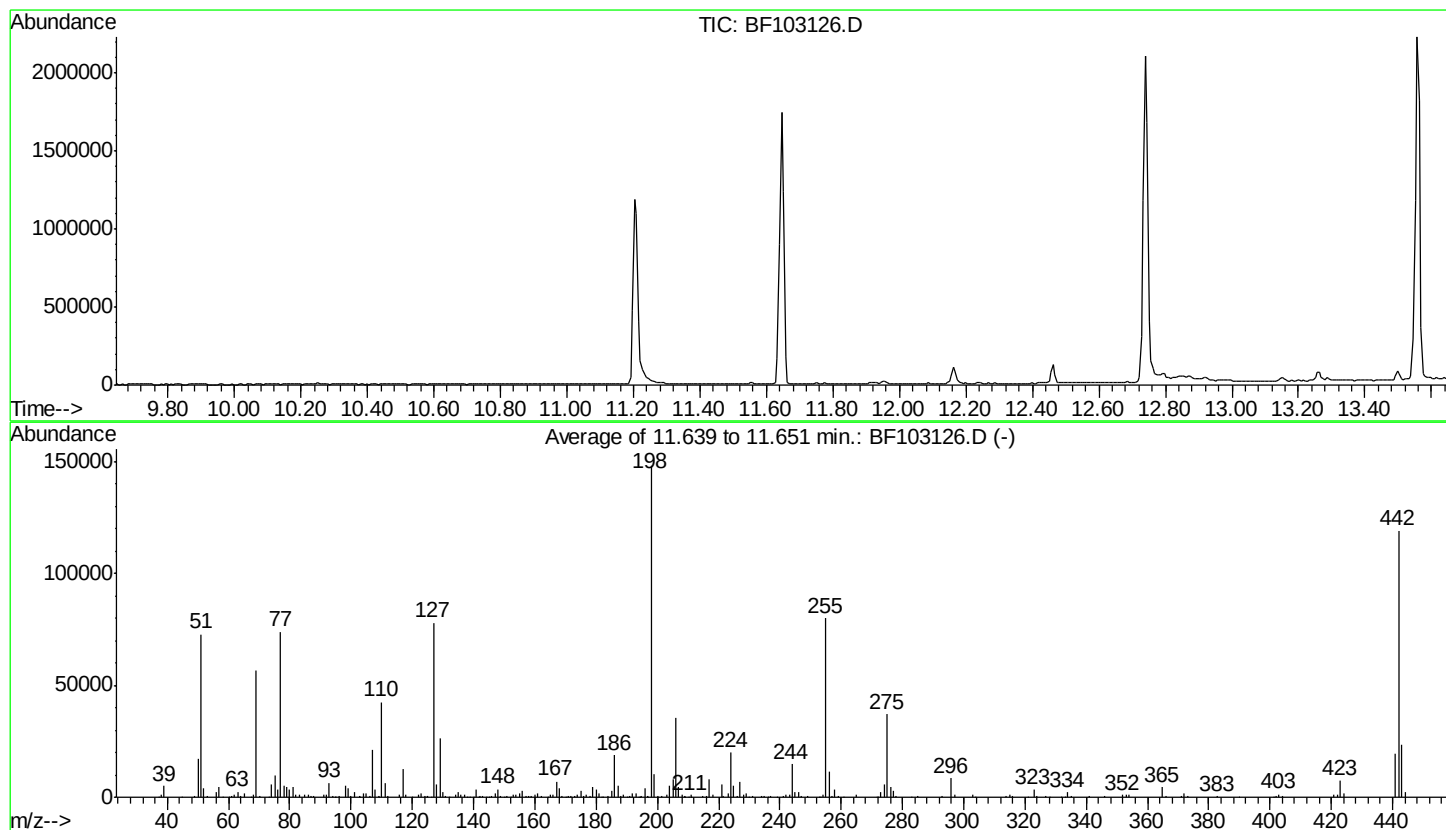

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.1	72645	PASS
68	69	0.00	2	1.8	1045	PASS
69	198	0.00	100	38.4	56781	PASS
70	69	0.00	2	0.7	372	PASS
127	198	10	80	52.6	77917	PASS
197	198	0.00	2	0.4	533	PASS
198	198	100	100	100.0	148016	PASS
199	198	5	9	6.9	10205	PASS
275	198	10	60	24.9	36922	PASS
365	198	1	100	2.9	4348	PASS
441	443	0.01	100	83.2	19610	PASS
442	198	50	100	80.4	119042	PASS
443	442	15	24	19.8	23568	PASS