
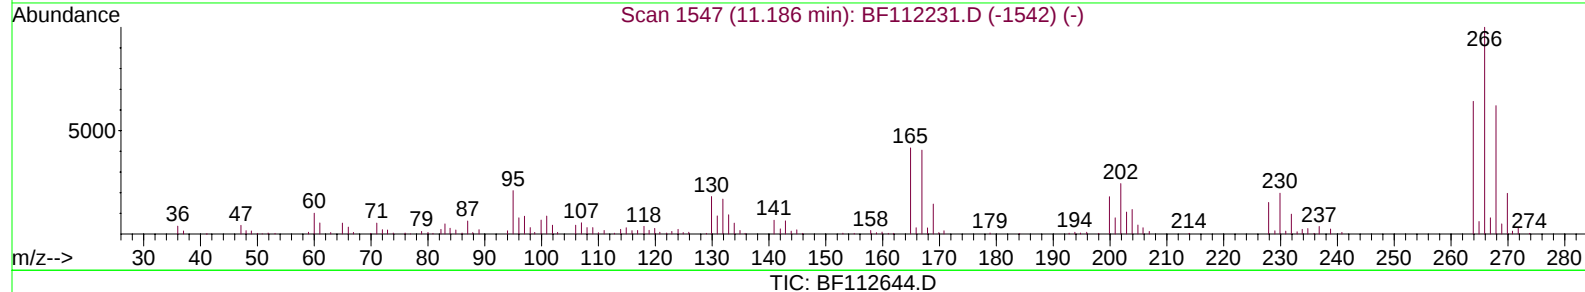
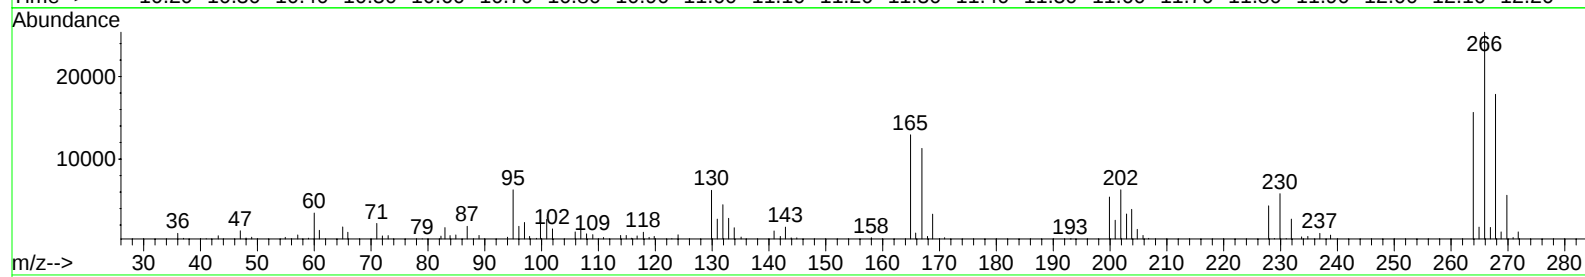


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF022119\
Data File : BF112644.D
Acq On : 21 Feb 2019 11:22
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 17:59:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

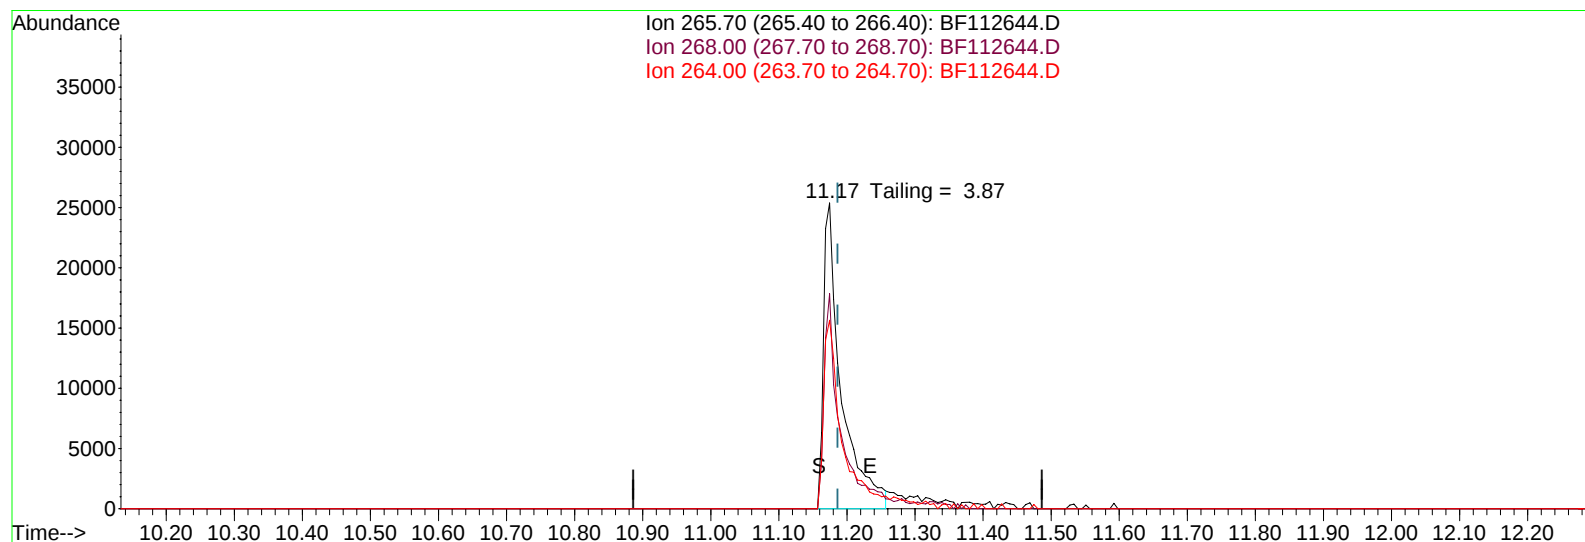

(70) Pentachlorophenol (C)




11.175min (-0.012) 67356.21ng

response 47954

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	70.31
264.00	63.60	61.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF022119\
 Data File : BF112644.D
 Acq On : 21 Feb 2019 11:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 17:59:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration

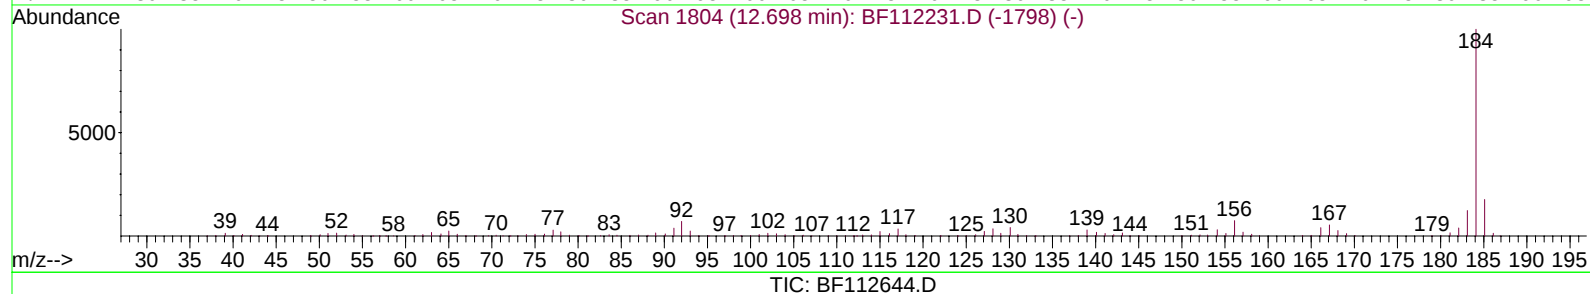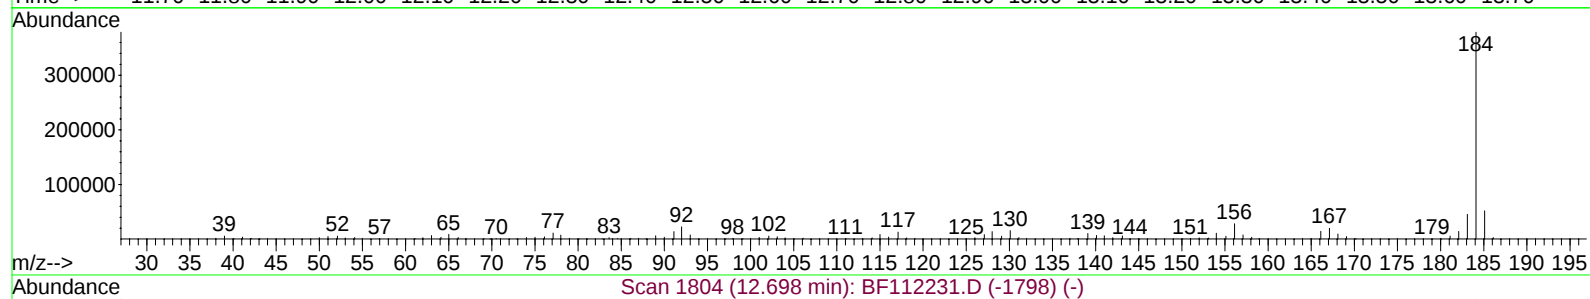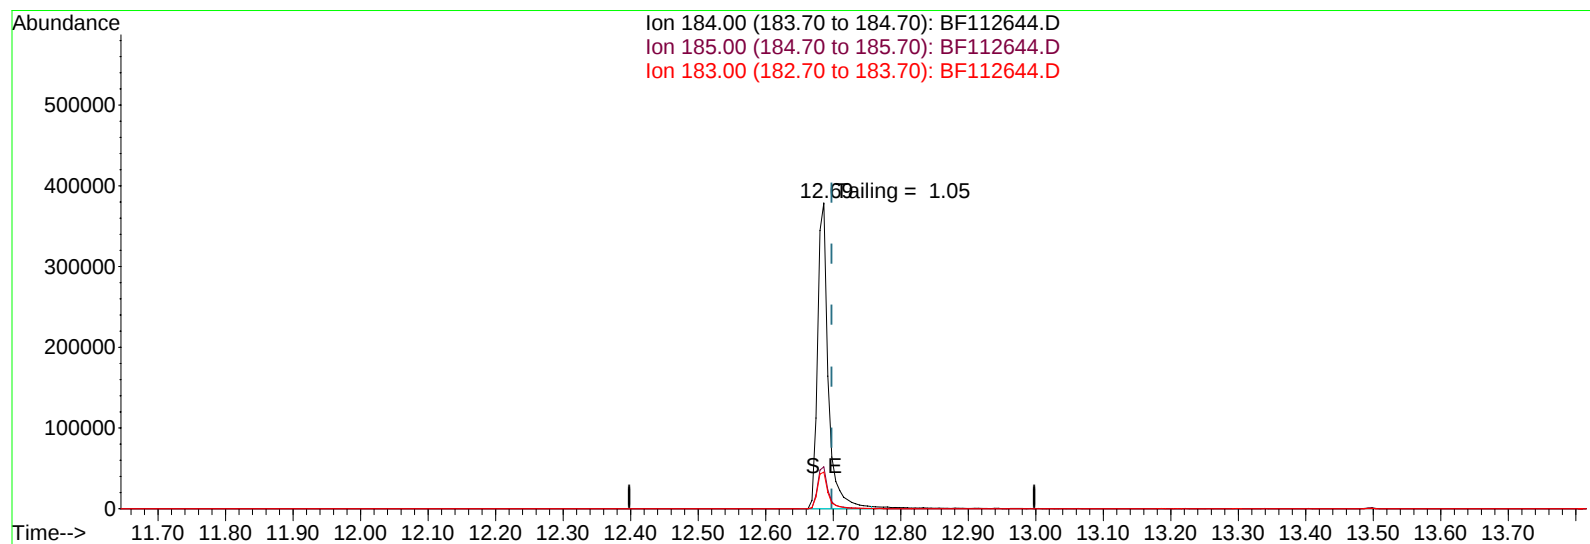

(77) Benzidine

12.686min (-0.012) 0.00ng

response 424025

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	13.71#
183.00	12.50	11.98
0.00	0.00	0.00