
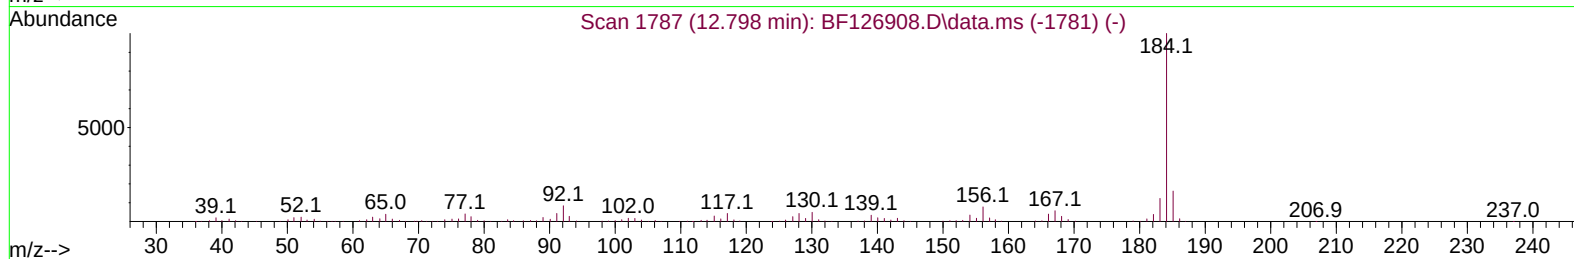
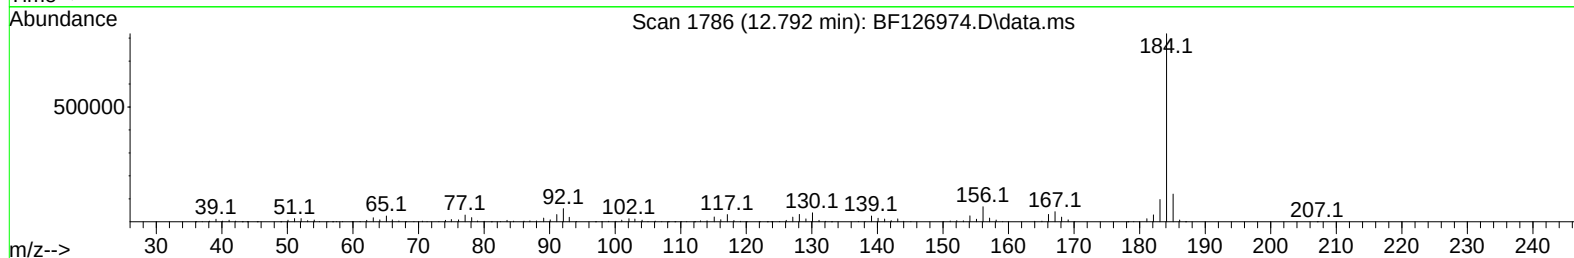


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022122\
Data File : BF126974.D
Acq On : 21 Feb 2022 15:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 17:15:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 21 13:16:57 2022
Response via : Initial Calibration

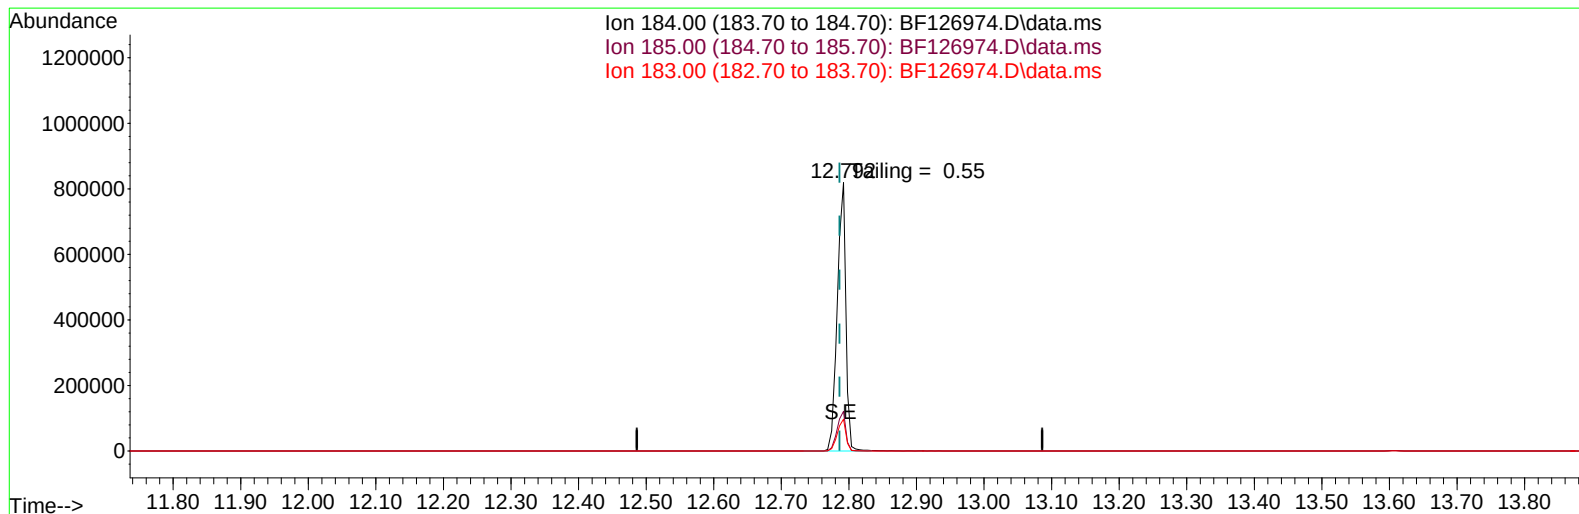

TIC: BF126974.D\data.ms

(77) Benzidine

12.792min (+ 0.006) 0.00 ng

response 721647

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.78
183.00	10.20	11.89
0.00	0.00	0.00