
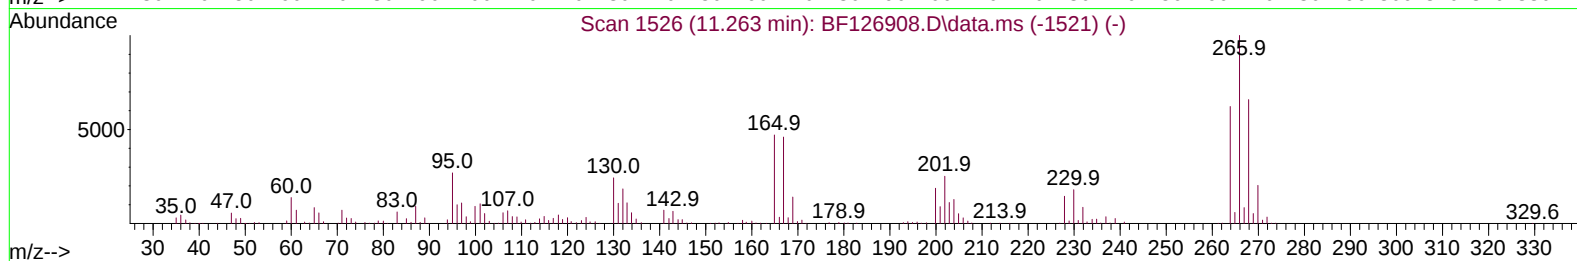
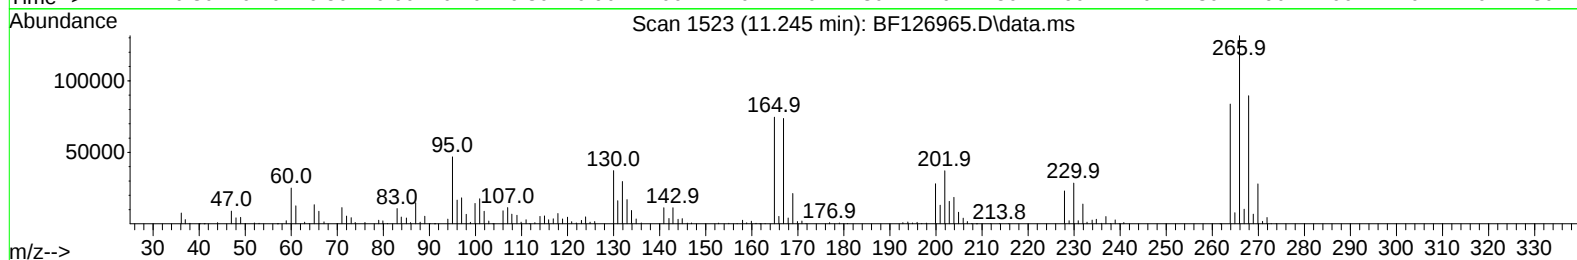


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022122\
Data File : BF126965.D
Acq On : 21 Feb 2022 10:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 13:12:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 16 14:55:48 2022
Response via : Initial Calibration

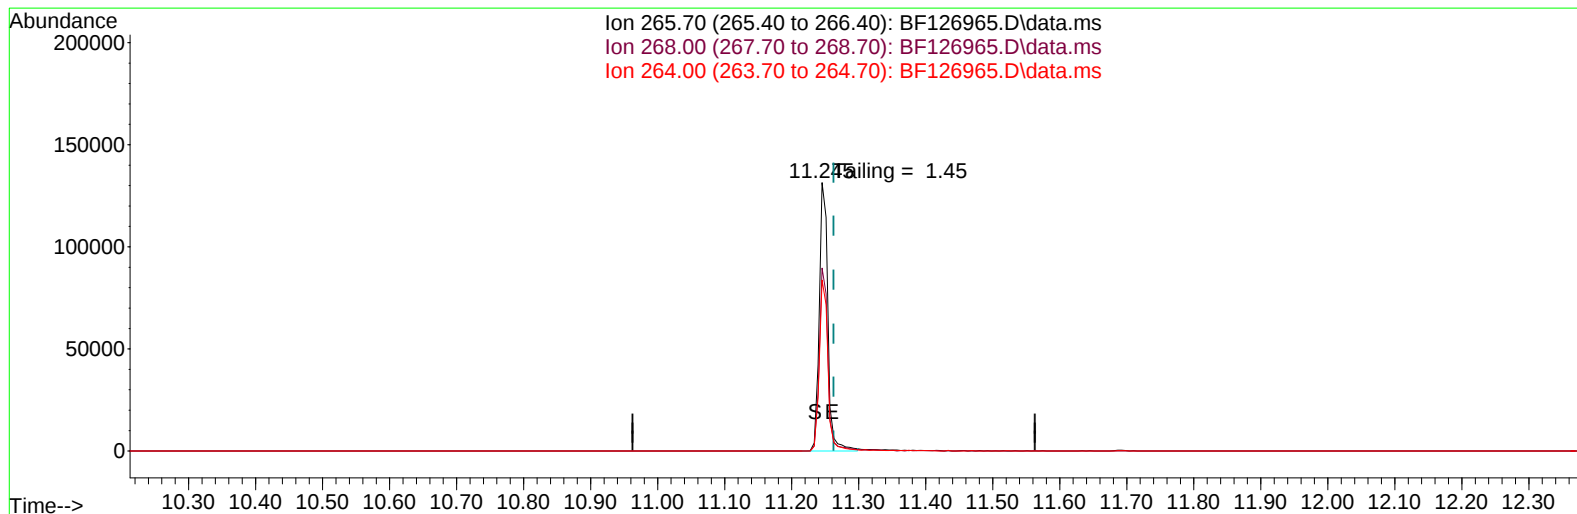

TIC: BF126965.D\data.ms

(70) Pentachlorophenol (C)




11.245min (-0.017) 22890.87 ng

response 119940

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	68.15
264.00	63.00	63.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022122\
Data File : BF126965.D
Acq On : 21 Feb 2022 10:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 13:12:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 16 14:55:48 2022
Response via : Initial Calibration

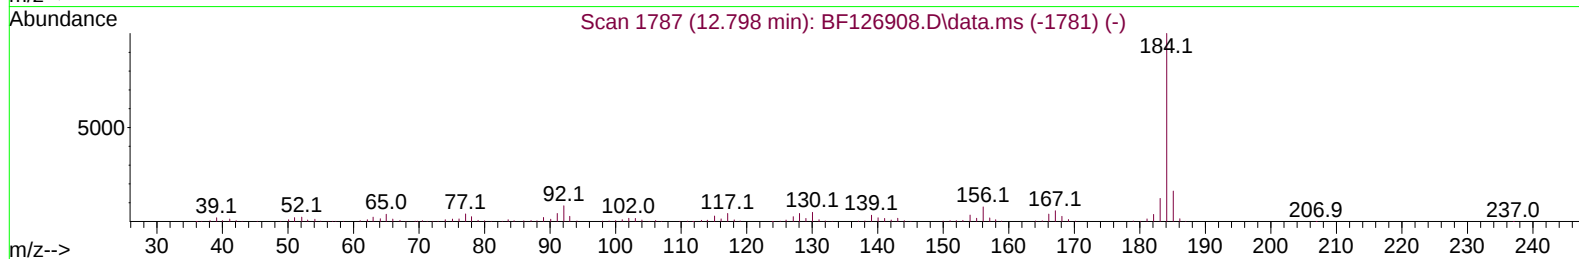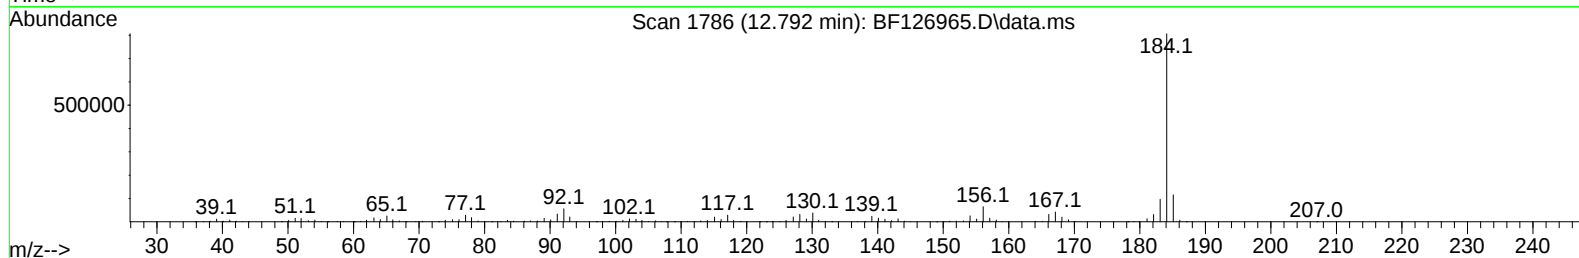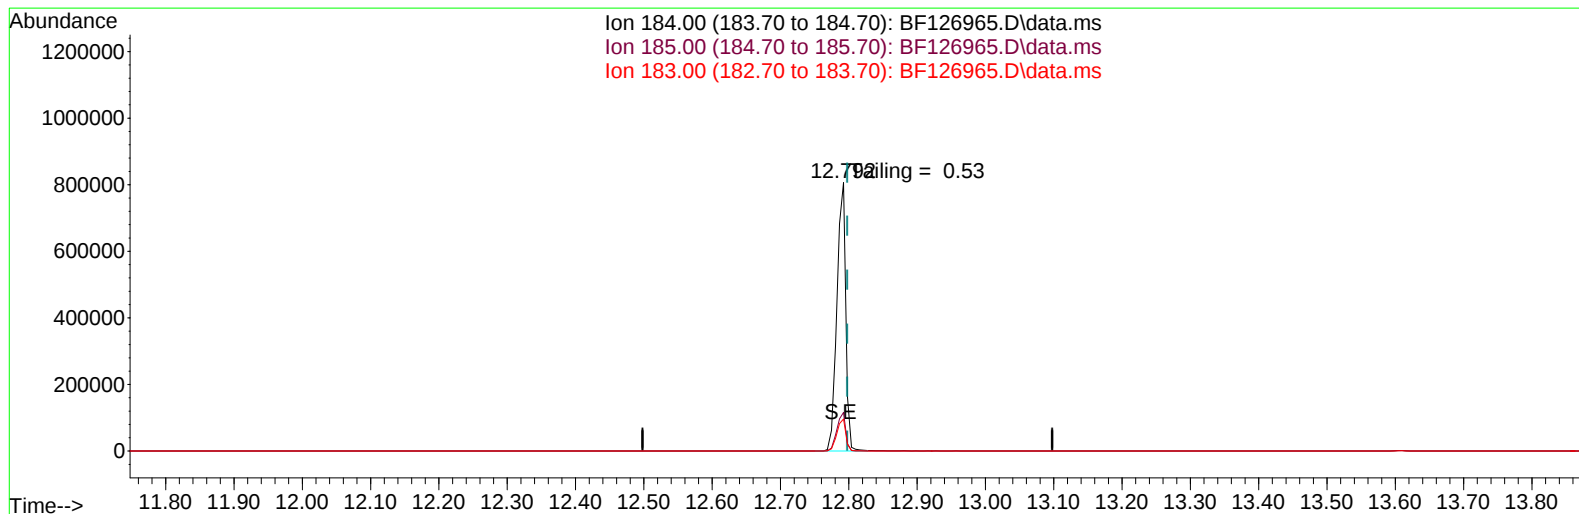

TIC: BF126965.D\data.ms

(77) Benzidine

12.792min (-0.006) 0.00 ng

response 728671

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.35
183.00	10.20	11.96
0.00	0.00	0.00