
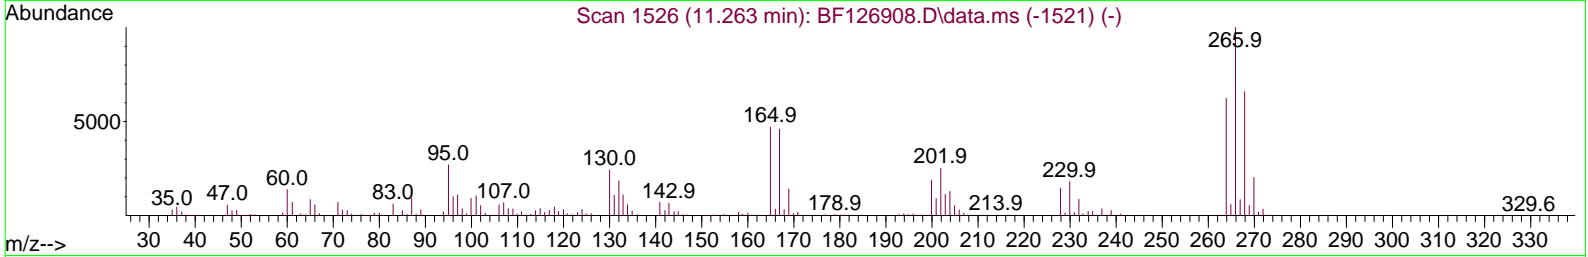
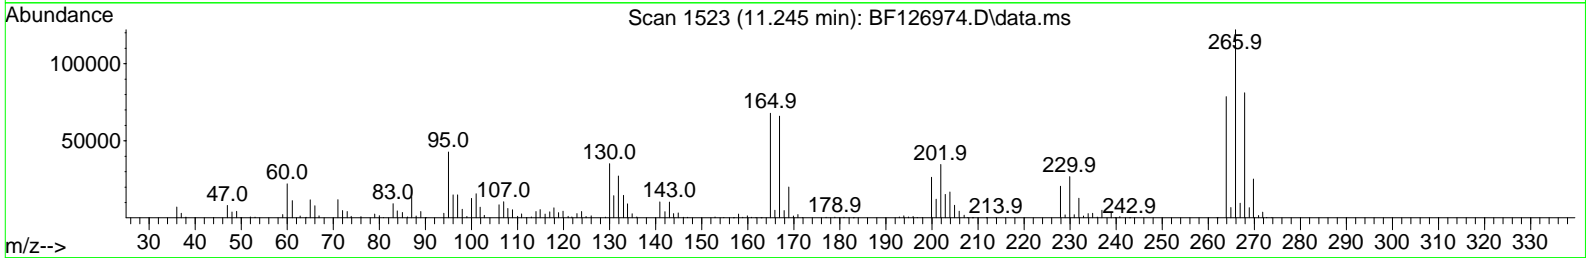


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022122\
 Data File : BF126974.D
 Acq On : 21 Feb 2022 15:28
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 17:15:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 21 13:16:57 2022
 Response via : Initial Calibration

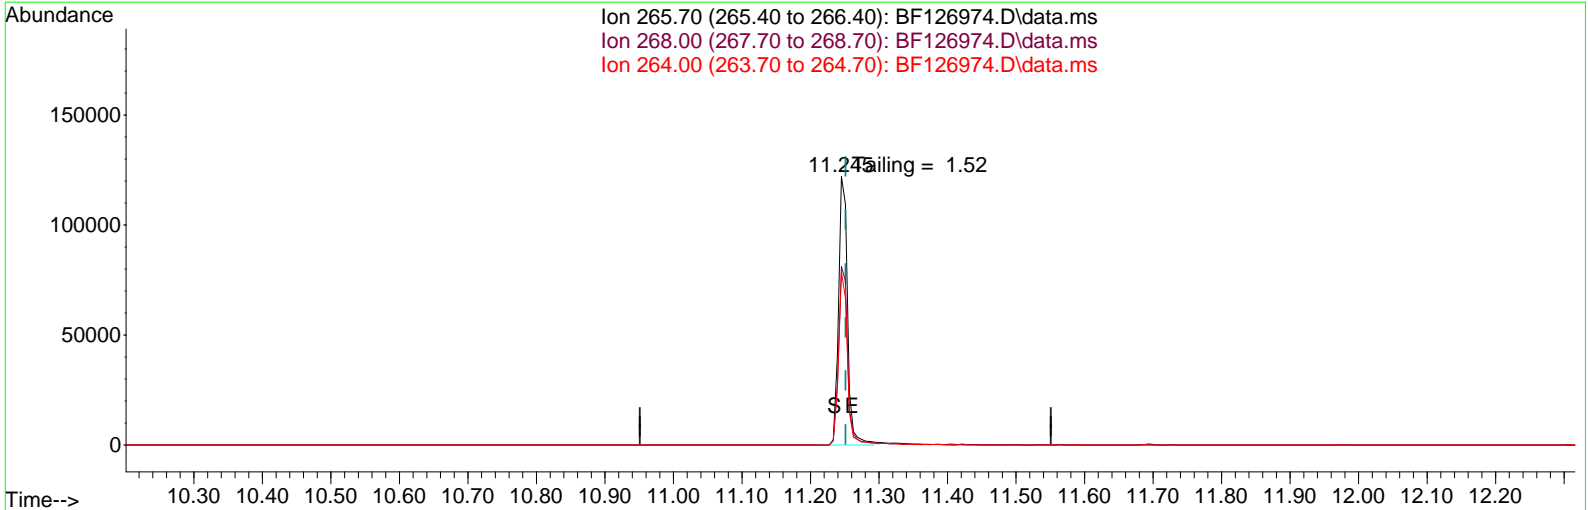

TIC: BF126974.D\data.ms

(70) Pentachlorophenol (C)

11.245min (-0.006) 27753.87 ng

response 112801

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.50
264.00	63.00	64.44
0.00	0.00	0.00

