

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022122\
 Data File : BF126986.D
 Acq On : 21 Feb 2022 21:16
 Operator : CG\JU
 Sample : N1602-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SPLP-LEACHATE-AMENDED-4A-COMP

Quant Time: Feb 22 03:52:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 21 13:16:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.916	152	89719	20.000	ng	0.00
21) Naphthalene-d8	8.198	136	366316	20.000	ng	# 0.00
39) Acenaphthene-d10	9.957	164	189126	20.000	ng	0.00
64) Phenanthrene-d10	11.445	188	325614	20.000	ng	# 0.00
76) Chrysene-d12	14.086	240	147525	20.000	ng	#-0.01
86) Perylene-d12	15.586	264	164394	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.540	112	445106	76.678	ng	0.00
7) Phenol-d6	6.534	99	410546	52.413	ng	-0.01
23) Nitrobenzene-d5	7.481	82	857672	105.682	ng	-0.01
42) 2,4,6-Tribromophenol	10.745	330	299416	137.503	ng	0.00
45) 2-Fluorobiphenyl	9.275	172	1381407	107.529	ng	0.00
79) Terphenyl-d14	13.033	244	1331271	132.657	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022122\
Data File : BF126986.D
Acq On : 21 Feb 2022 21:16
Operator : CG\JU
Sample : N1602-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SPLP-LEACHATE-AMENDED-4A-COMP

Quant Time: Feb 22 03:52:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 21 13:16:57 2022
Response via : Initial Calibration




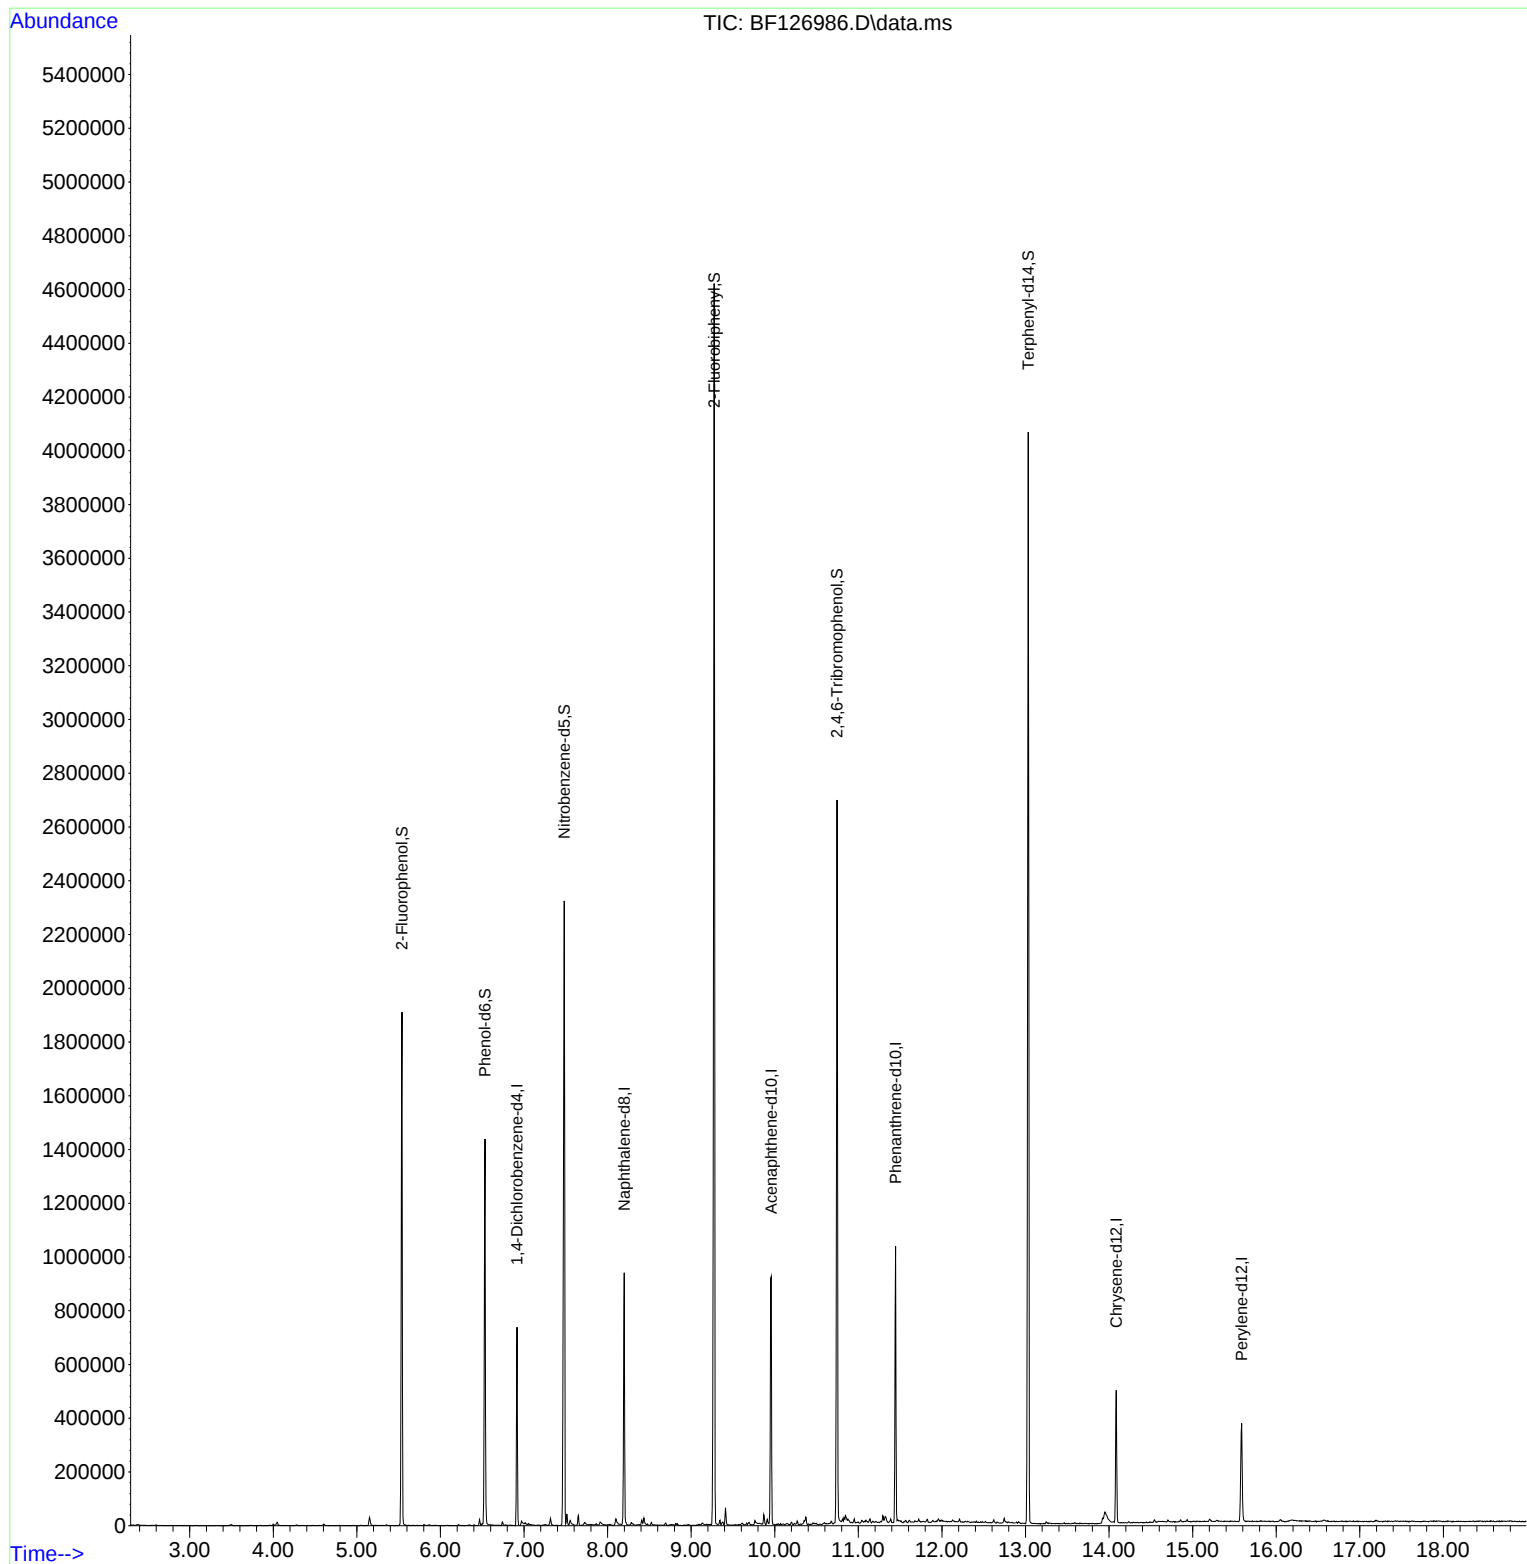




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.916 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF126986.D
Acq: 21 Feb 2022 21:16




Instrument :
BNA_F
ClientSampleId :
SPLP-LEACHATE-AMENDED-4A-COMP


Tgt Ion:152 Resp: 89719
Ion Ratio Lower Upper
152 100
150 152.5 128.1 192.1
115 66.9 56.7 85.1

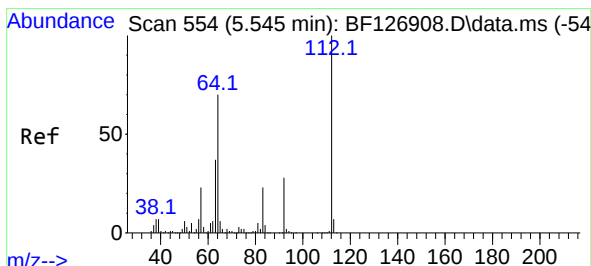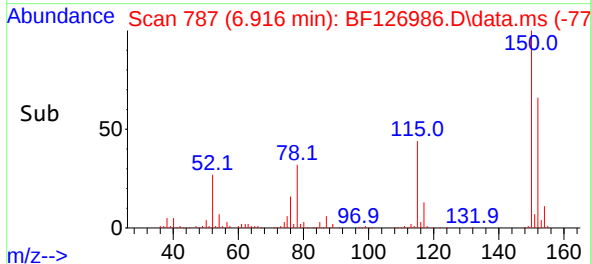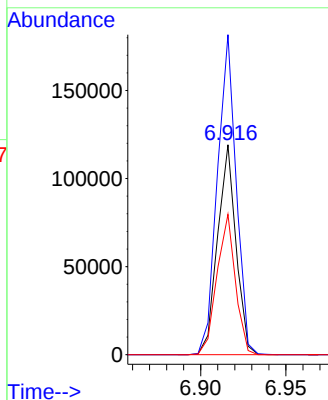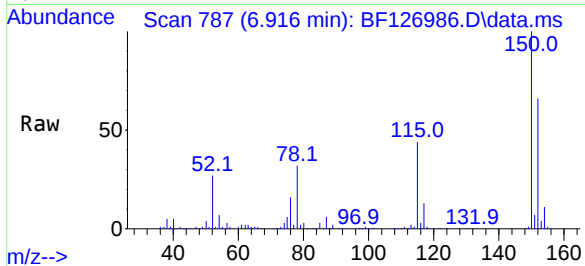

#5
2-Fluorophenol
Concen: 76.678 ng
RT: 5.540 min Scan# 553
Delta R.T. 0.000 min
Lab File: BF126986.D
Acq: 21 Feb 2022 21:16

Tgt Ion:112 Resp: 445106
Ion Ratio Lower Upper
112 100
64 66.8 49.5 74.3
63 35.6 23.9 35.9


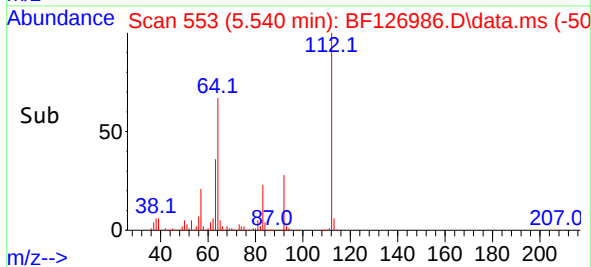
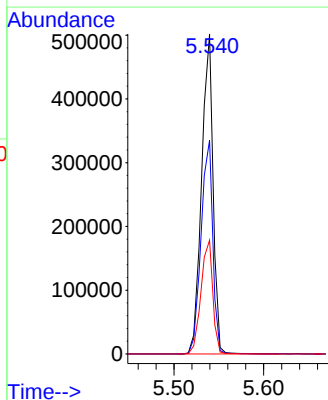
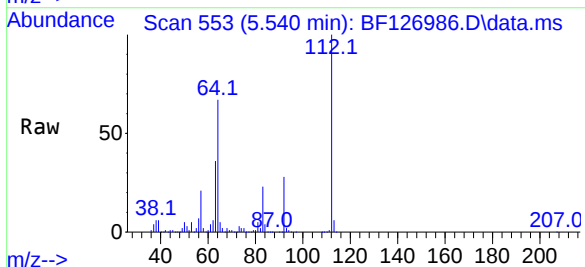


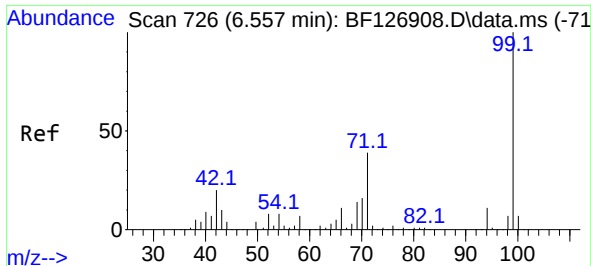

#7
Phenol-d6
Concen: 52.413 ng
RT: 6.534 min Scan# 71
Delta R.T. -0.012 min
Lab File: BF126986.D
Acq: 21 Feb 2022 21:16




Instrument :
BNA_F
ClientSampleId :
SPLP-LEACHATE-AMENDED-4A-COMP

Tgt Ion: 99 Resp: 410546
Ion Ratio Lower Upper
99 100
42 19.4 14.2 21.4
71 39.5 24.3 36.5#

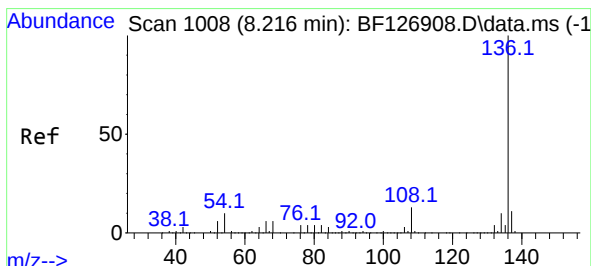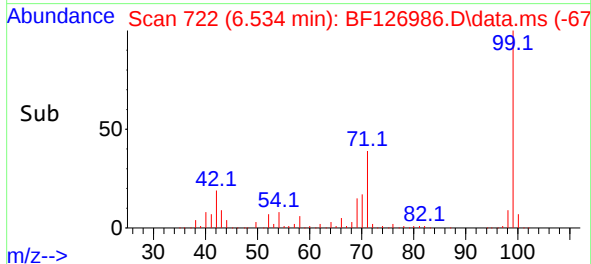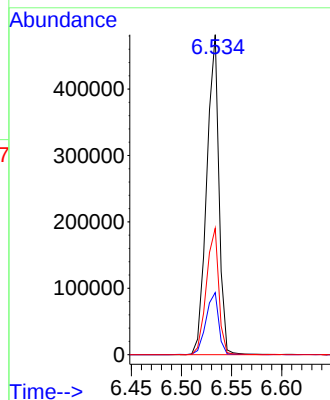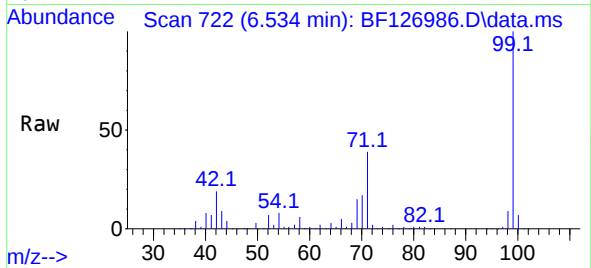

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.198 min Scan# 1005
Delta R.T. -0.006 min
Lab File: BF126986.D
Acq: 21 Feb 2022 21:16

Tgt Ion:136 Resp: 366316
Ion Ratio Lower Upper
136 100
137 10.6 8.6 13.0
54 8.4 7.8 11.6
68 5.0 6.3 9.5#

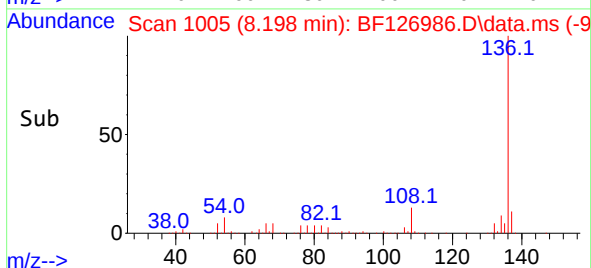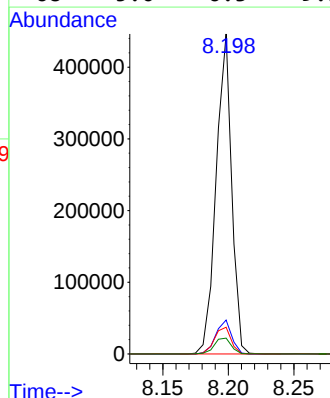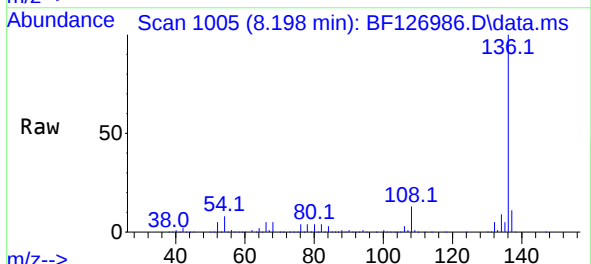



#23

Nitrobenzene-d5

Concen: 105.682 ng

RT: 7.481 min Scan# 81

Delta R.T. -0.012 min

Lab File: BF126986.D

Acq: 21 Feb 2022 21:16

Instrument :





BNA_F

ClientSampleId :

SPLP-LEACHATE-AMENDED-4A-COMP

Tgt Ion: 82 Resp: 857672

Ion	Ratio	Lower	Upper
82	100		
128	38.1	32.7	49.1
54	53.4	41.7	62.5

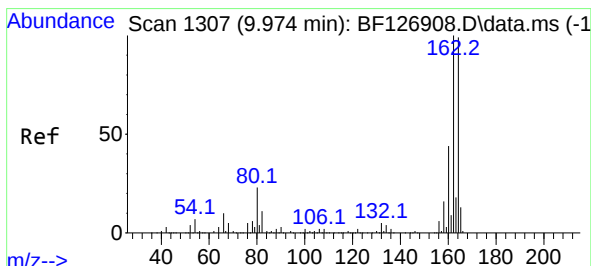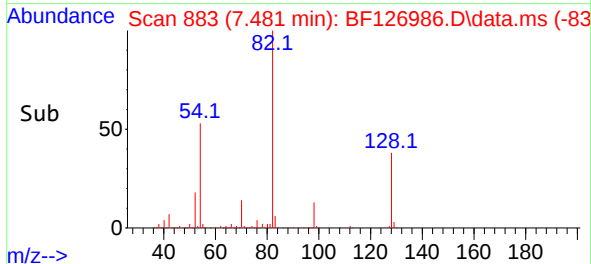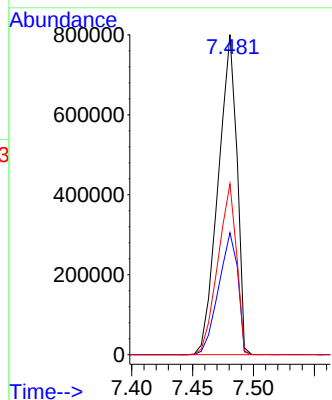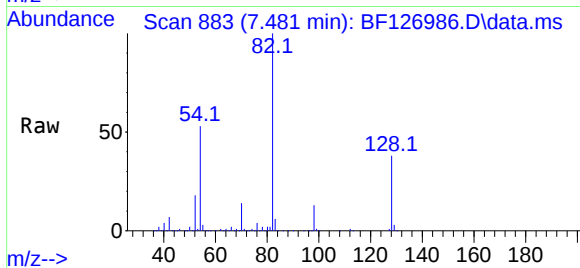

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.957 min Scan# 1304




Delta R.T. -0.006 min

Lab File: BF126986.D

Acq: 21 Feb 2022 21:16

Tgt Ion: 164 Resp: 189126

Ion	Ratio	Lower	Upper
164	100		
162	100.1	81.4	122.0
160	44.4	36.6	54.8

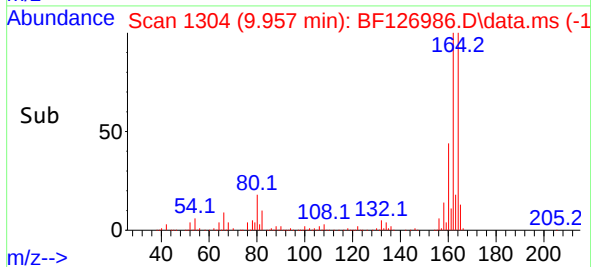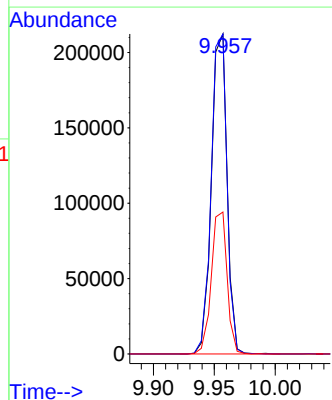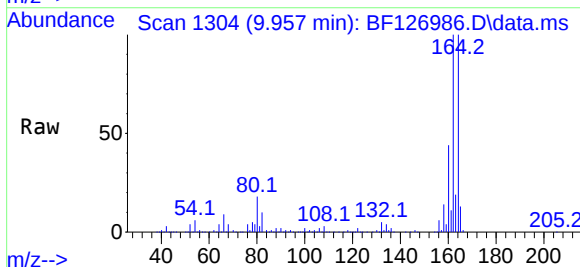



#42

2,4,6-Tribromophenol

Concen: 137.503 ng

RT: 10.745 min Scan# 1442

Delta R.T. -0.006 min

Lab File: BF126986.D


Acq: 21 Feb 2022 21:16

Instrument :

BNA_F

ClientSampleId :

SPLP-LEACHATE-AMENDED-4A-COMP

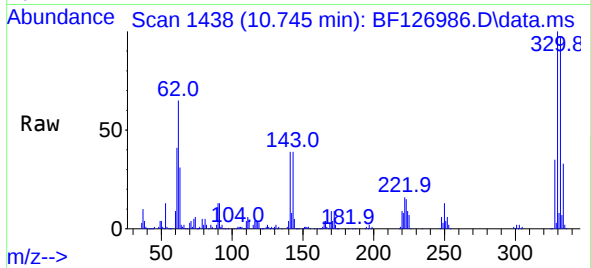




Tgt Ion:330 Resp: 299416

Ion Ratio Lower Upper

330 100

332 97.0 76.0 114.0

141 35.8 30.1 45.1

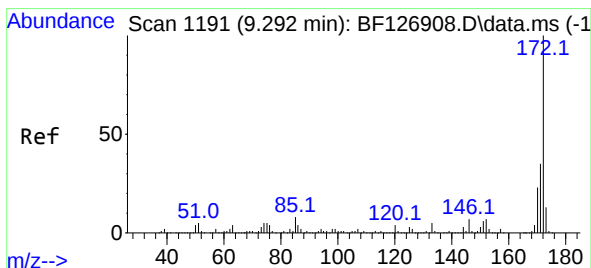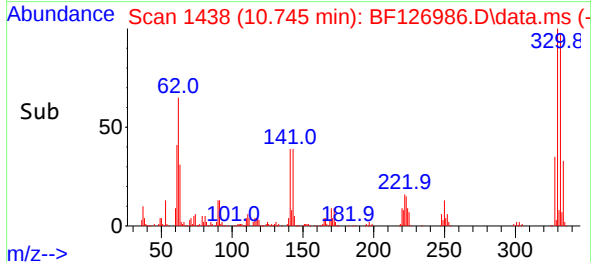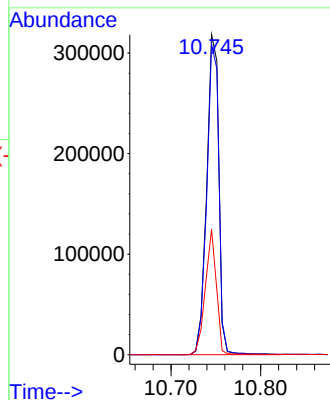

#45

2-Fluorobiphenyl

Concen: 107.529 ng

RT: 9.275 min Scan# 1188

Delta R.T. -0.006 min

Lab File: BF126986.D

Acq: 21 Feb 2022 21:16




Tgt Ion:172 Resp: 1381407

Ion Ratio Lower Upper

172 100

171 35.6 28.3 42.5

170 23.7 19.0 28.6


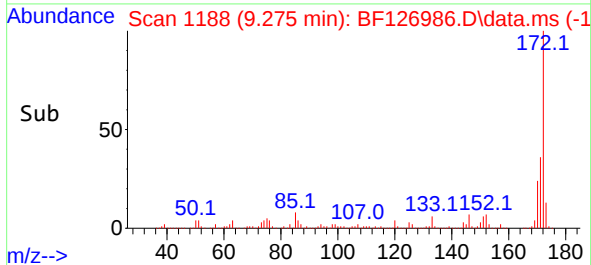
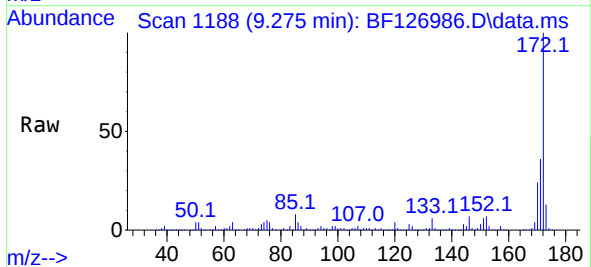
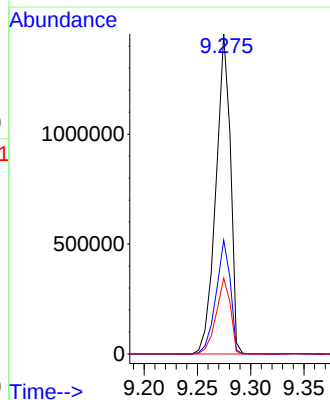




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.445 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF126986.D
Acq: 21 Feb 2022 21:16




Instrument :
BNA_F
ClientSampleId :
SPLP-LEACHATE-AMENDED-4A-COMP

Tgt Ion:188 Resp: 325614
Ion Ratio Lower Upper
188 100
94 8.7 10.1 15.1#
80 10.4 11.8 17.6#

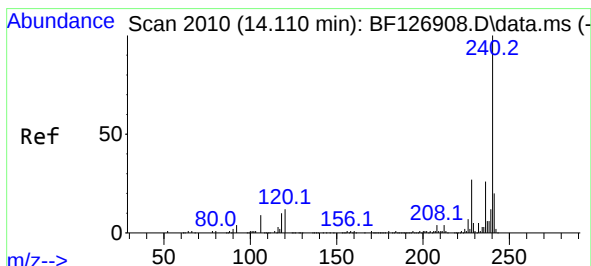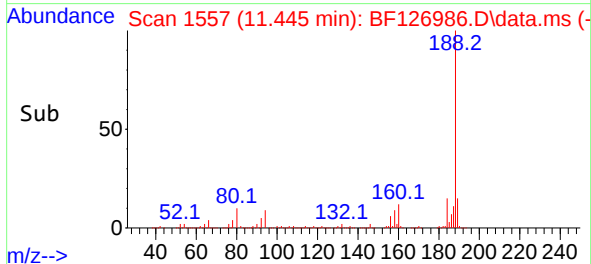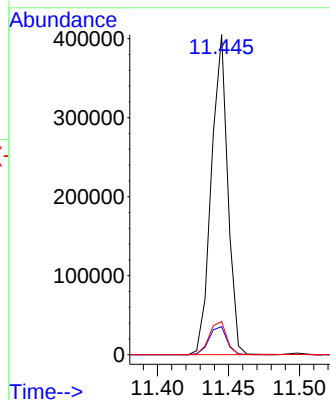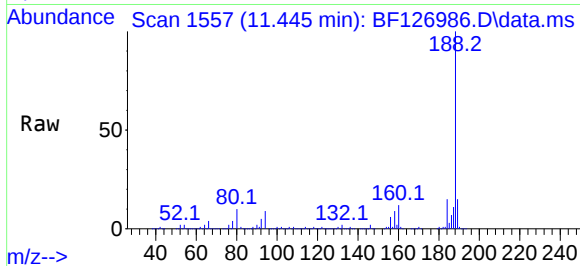

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.086 min Scan# 2006
Delta R.T. -0.012 min
Lab File: BF126986.D
Acq: 21 Feb 2022 21:16


Tgt Ion:240 Resp: 147525
Ion Ratio Lower Upper
240 100
120 10.4 14.4 21.6#
236 24.5 20.5 30.7

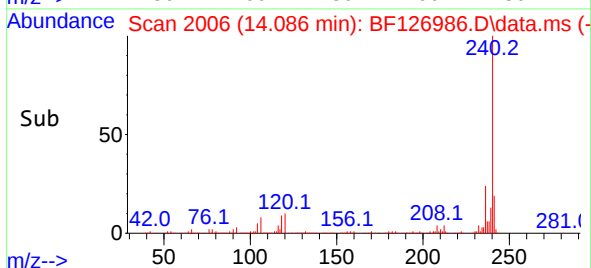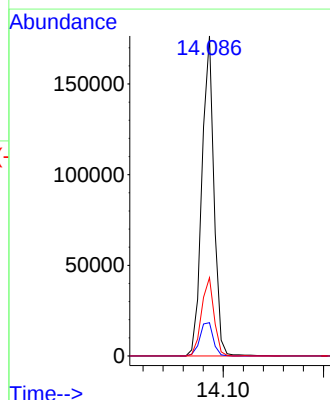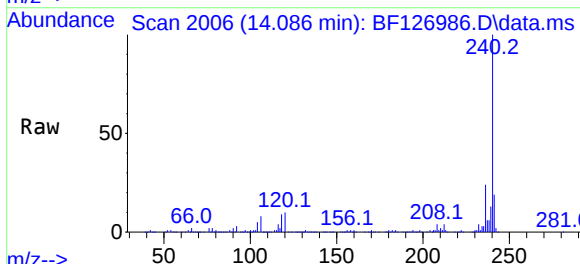






#79
 Terphenyl-d14
 Concen: 132.657 ng
 RT: 13.033 min Scan# 1827
 Delta R.T. -0.006 min
 Lab File: BF126986.D
 Acq: 21 Feb 2022 21:16

Instrument : BNA_F
 ClientSampleId : SPLP-LEACHATE-AMENDED-4A-COMP

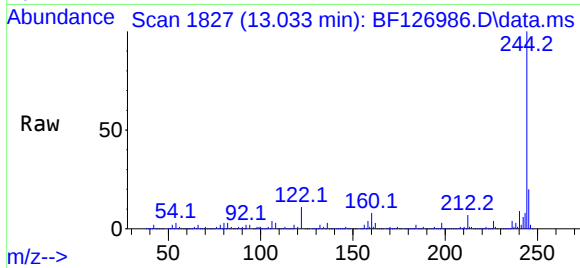

Tgt Ion:244 Resp: 1331271
 Ion Ratio Lower Upper
 244 100
 212 7.0 5.0 7.4
 122 11.4 13.3 19.9#

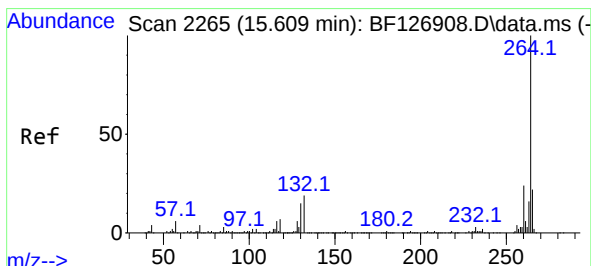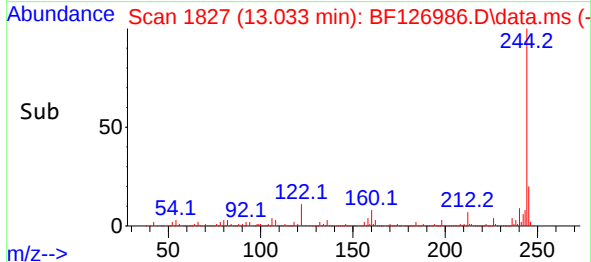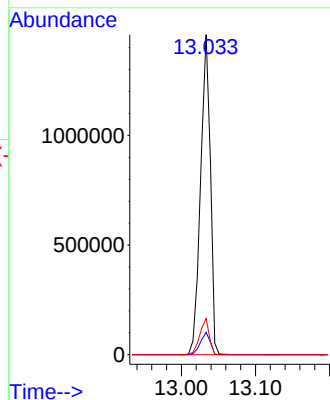

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.586 min Scan# 2261
 Delta R.T. -0.006 min
 Lab File: BF126986.D
 Acq: 21 Feb 2022 21:16

Tgt Ion:264 Resp: 164394
 Ion Ratio Lower Upper
 264 100
 260 24.1 19.2 28.8
 265 21.2 17.4 26.2

