

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022122\
 Data File : BF126968.D
 Acq On : 21 Feb 2022 12:22
 Operator : CG\JU
 Sample : PB142473BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB142473BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126968.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.551	550	555	558	rBV	3232843	3208166	74.63%	12.817%
2	6.545	718	724	727	rBV	3025920	3269324	76.05%	13.062%
3	6.922	784	788	791	rBV	778179	666268	15.50%	2.662%
4	7.487	878	884	887	rBV	2012531	2245043	52.22%	8.969%
5	8.198	1000	1005	1009	rBV	910523	893458	20.78%	3.570%
6	9.281	1182	1189	1192	rBV	4088180	3845209	89.44%	15.362%
7	9.957	1299	1304	1308	rBV	1108633	959857	22.33%	3.835%
8	10.751	1434	1439	1442	rBV	2868401	2561810	59.59%	10.235%
9	11.451	1554	1558	1561	rVB	1111620	1010116	23.50%	4.036%
10	12.845	1792	1795	1798	rBV	94934	68167	1.59%	0.272%
11	13.039	1823	1828	1831	rBV	4745757	4299026	100.00%	17.175%
12	13.551	1912	1915	1919	rBV	65294	49569	1.15%	0.198%
13	14.092	2003	2007	2010	rBV	1043301	895098	20.82%	3.576%
14	15.210	2193	2197	2205	rVB2	39146	47548	1.11%	0.190%
15	15.592	2256	2262	2275	rVB2	699309	913269	21.24%	3.649%
16	16.057	2337	2341	2346	rVB3	33233	50429	1.17%	0.201%
17	16.586	2426	2431	2439	rBV2	25977	47695	1.11%	0.191%


Sum of corrected areas: 25030052

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022122\
Data File : BF126968.D
Acq On : 21 Feb 2022 12:22
Operator : CG\JU
Sample : PB142473BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142473BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

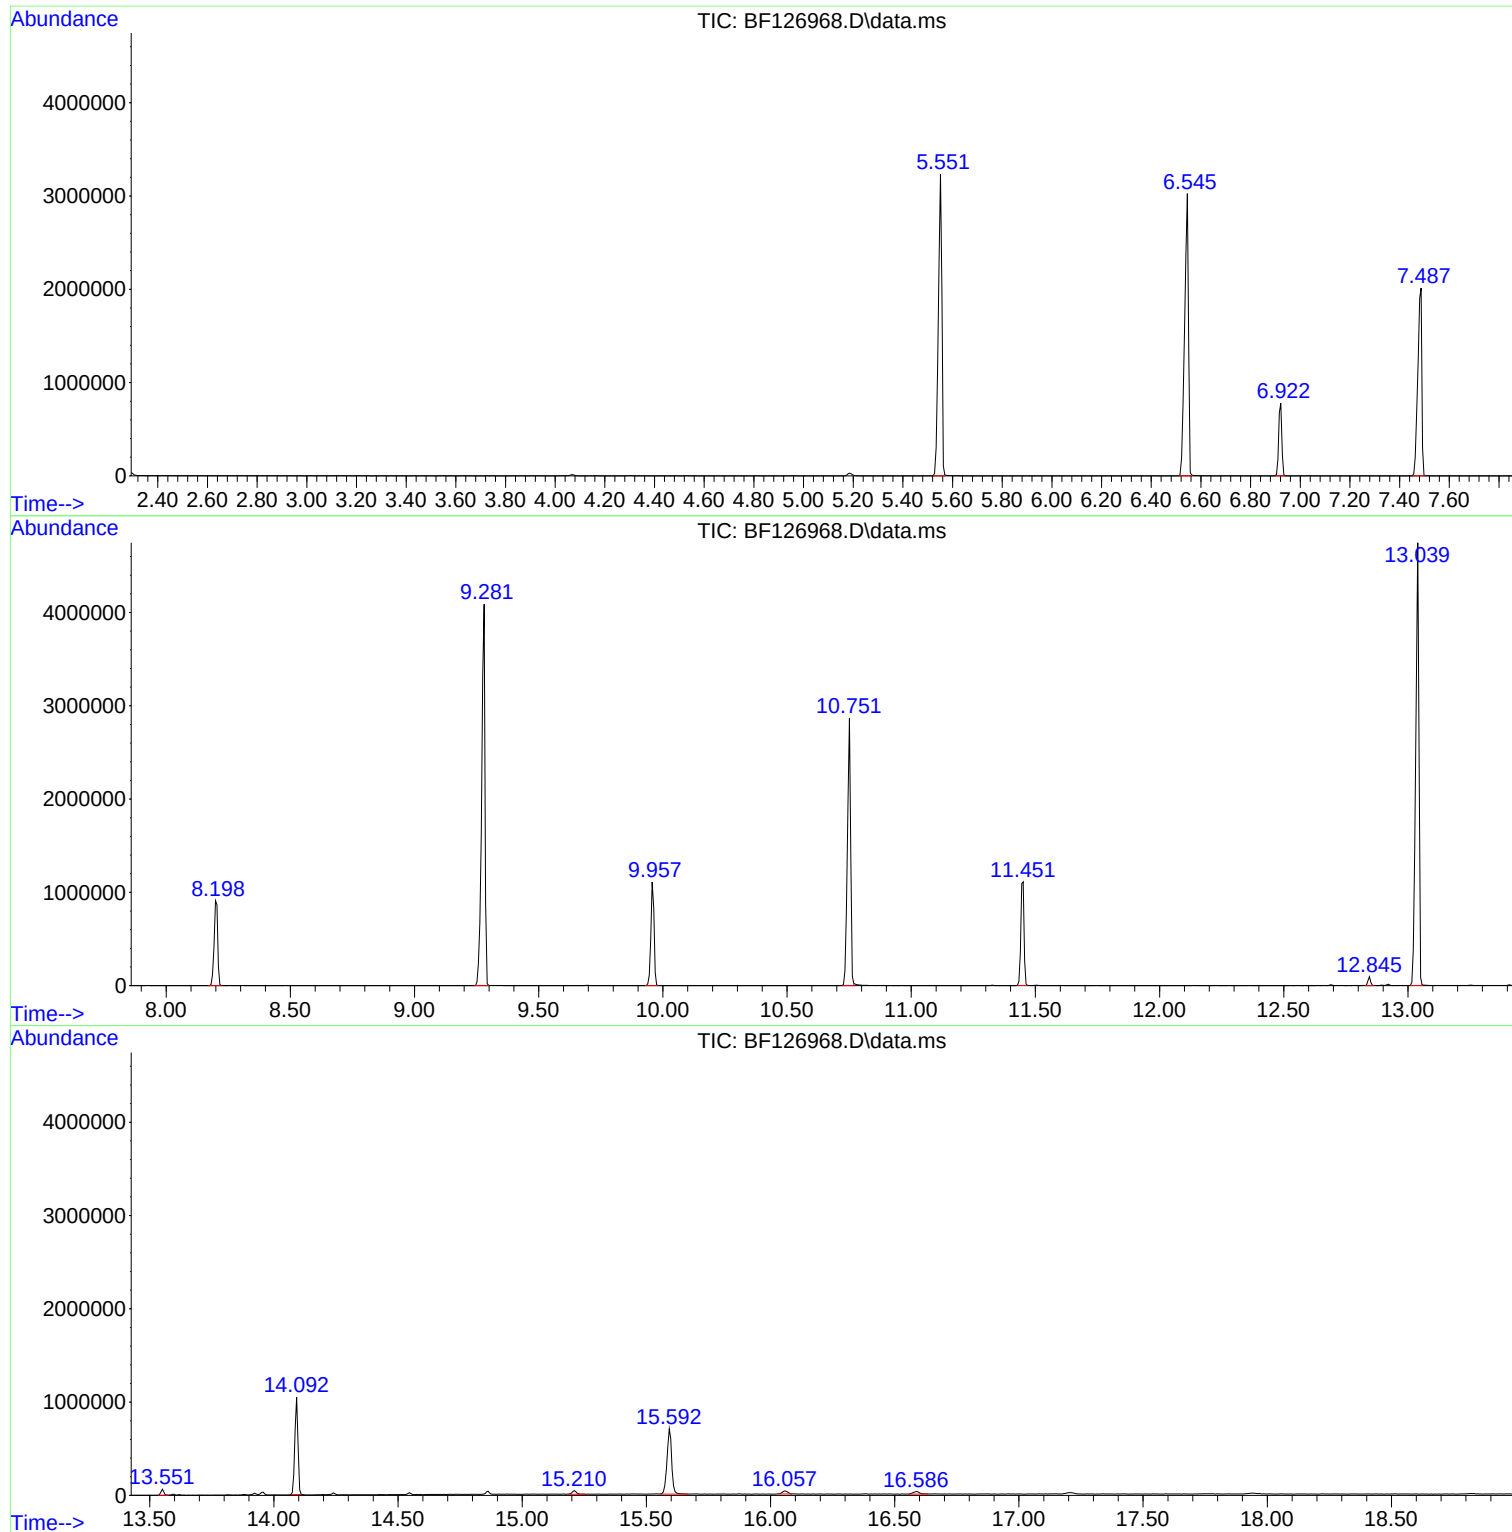

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022122\
Data File : BF126968.D
Acq On : 21 Feb 2022 12:22
Operator : CG\JU
Sample : PB142473BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142473BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022122\
Data File : BF126968.D
Acq On : 21 Feb 2022 12:22
Operator : CG\JU
Sample : PB142473BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142473BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------