

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022122\
 Data File : BF126983.D
 Acq On : 21 Feb 2022 19:51
 Operator : CG\JU
 Sample : N1579-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-6-(6.5-7.0)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126983.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.157	483	488	493	rBV	27445	34441	1.17%	0.198%
2	5.540	548	553	556	rBV	2606613	2366459	80.62%	13.608%
3	6.540	717	723	726	rBV	2360729	2498768	85.13%	14.369%
4	6.916	783	787	790	rBV	747062	570789	19.45%	3.282%
5	7.481	877	883	886	rBV	1608190	1672980	57.00%	9.620%
6	8.092	983	987	996	rBV	40989	60974	2.08%	0.351%
7	8.198	1000	1005	1008	rBV	899130	776800	26.46%	4.467%
8	9.275	1182	1188	1191	rBV	3442214	2935213	100.00%	16.879%
9	9.763	1268	1271	1280	rBV6	15309	35956	1.22%	0.207%
10	9.957	1299	1304	1307	rBV	961855	859932	29.30%	4.945%
11	10.745	1434	1438	1441	rBV	1274704	1168888	39.82%	6.722%
12	11.445	1553	1557	1560	rBV	1051984	859060	29.27%	4.940%
13	13.033	1822	1827	1830	rBV	2927971	2531645	86.25%	14.558%
14	13.951	1976	1983	1996	rBV7	28606	97377	3.32%	0.560%
15	14.086	2002	2006	2009	rBV	481111	412501	14.05%	2.372%
16	14.933	2147	2150	2157	rBV	36518	43512	1.48%	0.250%
17	15.586	2255	2261	2266	rBV	353785	464523	15.83%	2.671%




Sum of corrected areas: 17389818

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022122\
Data File : BF126983.D
Acq On : 21 Feb 2022 19:51
Operator : CG\JU
Sample : N1579-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-6-(6.5-7.0)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

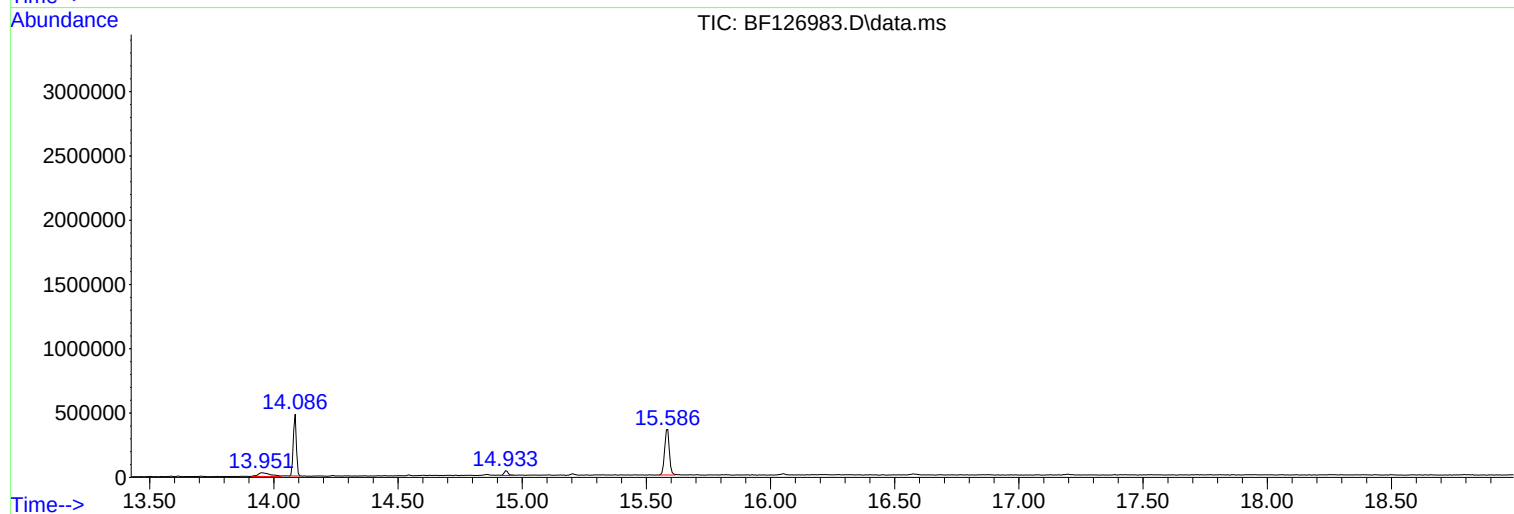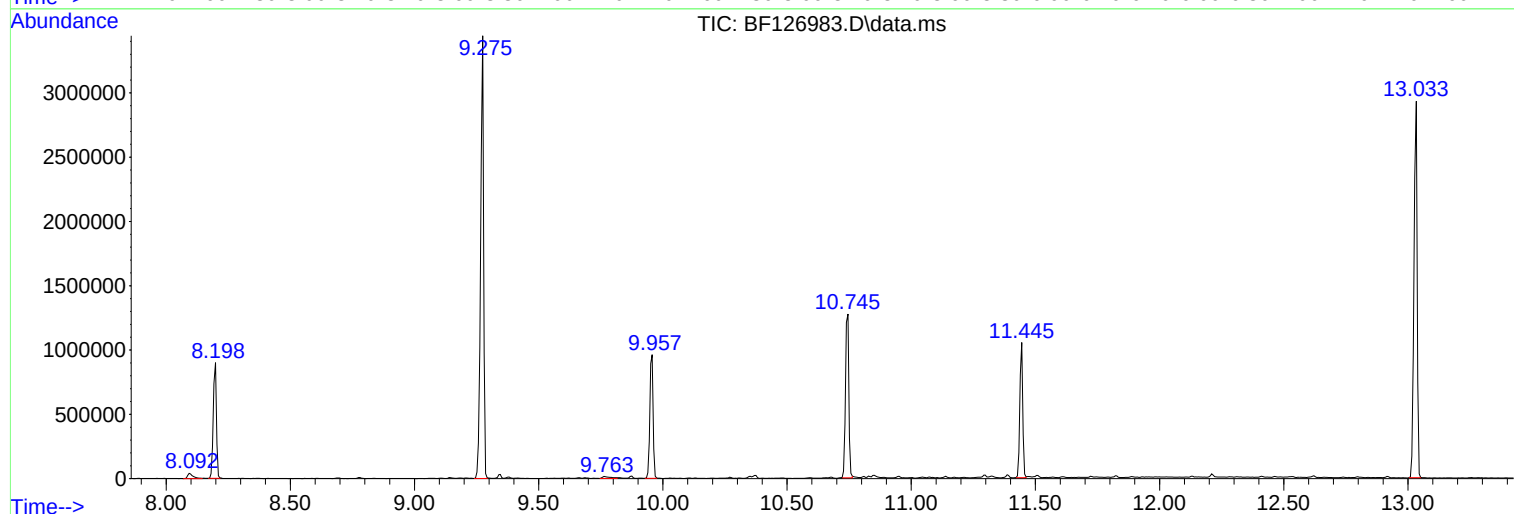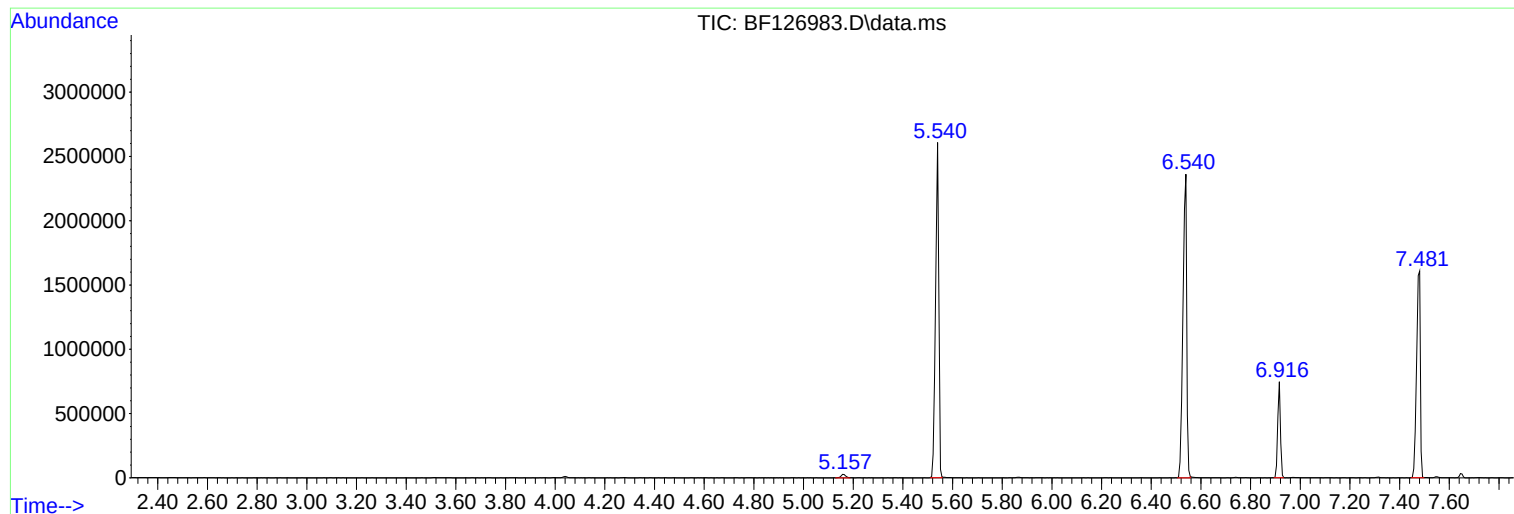

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022122\
Data File : BF126983.D
Acq On : 21 Feb 2022 19:51
Operator : CG\JU
Sample : N1579-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-6-(6.5-7.0)










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Octadecanol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.951	4.72 ng	97377	Chrysene-d12	14.086

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Octadecanol	270	C18H38O	000112-92-5	80
2			n-Heptadecanol-1	256	C17H36O	001454-85-9	80
3			Chloroacetic acid, tetradecyl ester	290	C16H31ClO2	018277-86-6	72
4			Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	72
5			Heptadecyl trifluoroacetate	352	C19H35F3O2	1010351-87-0	72

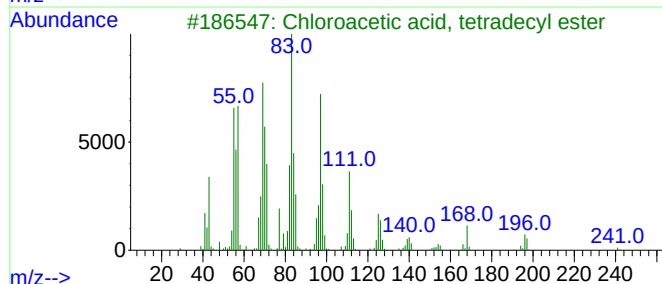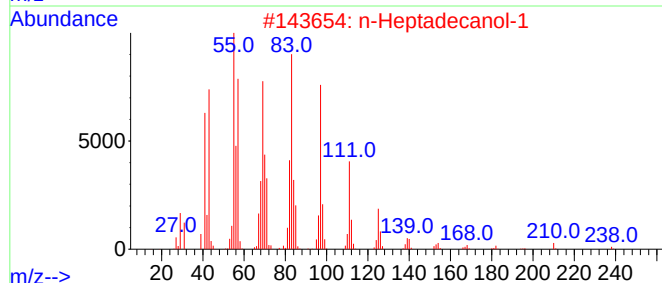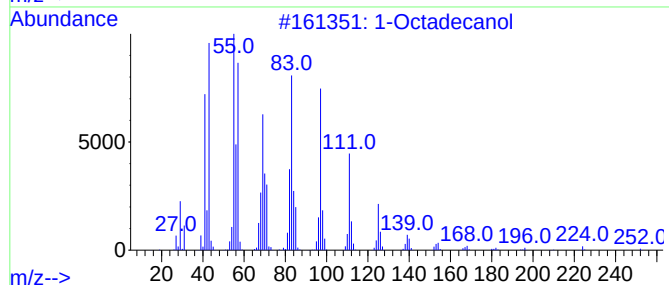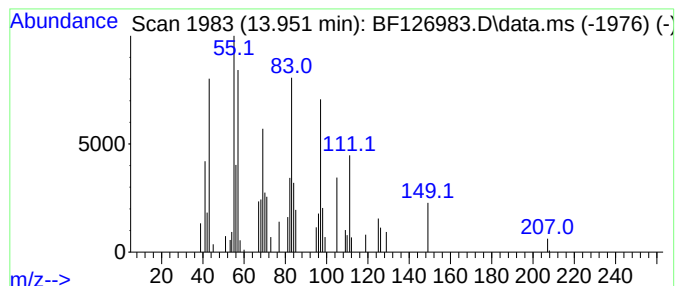

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022122\
Data File : BF126983.D
Acq On : 21 Feb 2022 19:51
Operator : CG\JU
Sample : N1579-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-6-(6.5-7.0)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Octadecanol	13.951	4.7	ng	97377	5	14.086	412501	20.0