
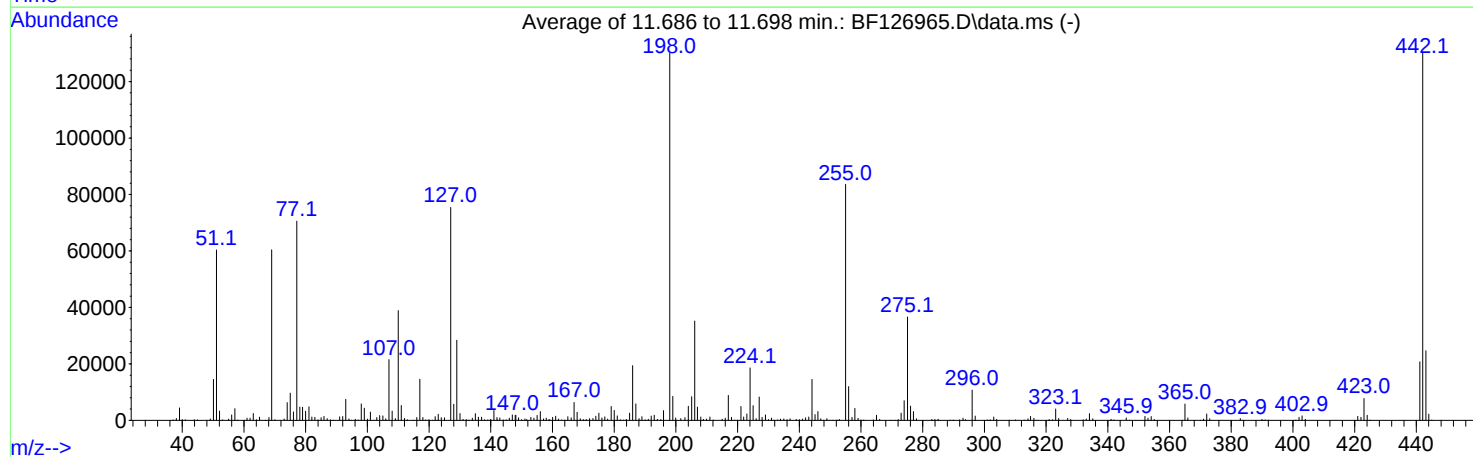


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022122\
 Data File : BF126965.D
 Acq On : 21 Feb 2022 10:59
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 21 13:16:57 2022

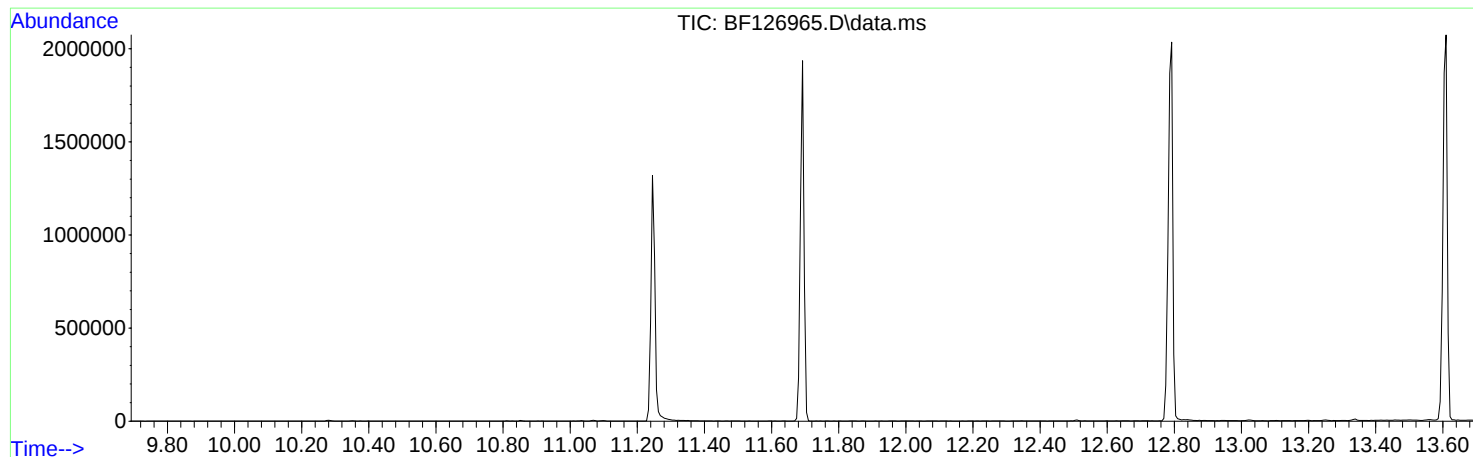




AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.4	60389	PASS
68	69	0.00	2	1.7	1009	PASS
69	198	0.00	100	46.5	60408	PASS
70	69	0.00	2	0.4	251	PASS
127	198	10	80	58.0	75461	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	130045	PASS
199	198	5	9	6.5	8504	PASS
275	198	10	60	28.2	36637	PASS
365	198	1	100	4.4	5762	PASS
441	198	0.01	100	15.9	20721	PASS
442	442	50	100	100.0	130299	PASS
443	442	15	24	18.9	24662	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022122\
Data File : BF126965.D
Acq On : 21 Feb 2022 10:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 21 13:12:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 16 14:55:48 2022
Response via : Initial Calibration

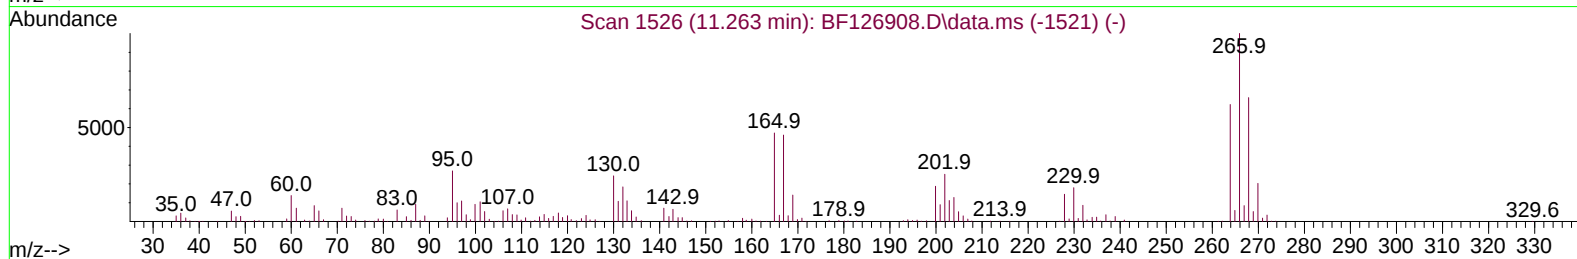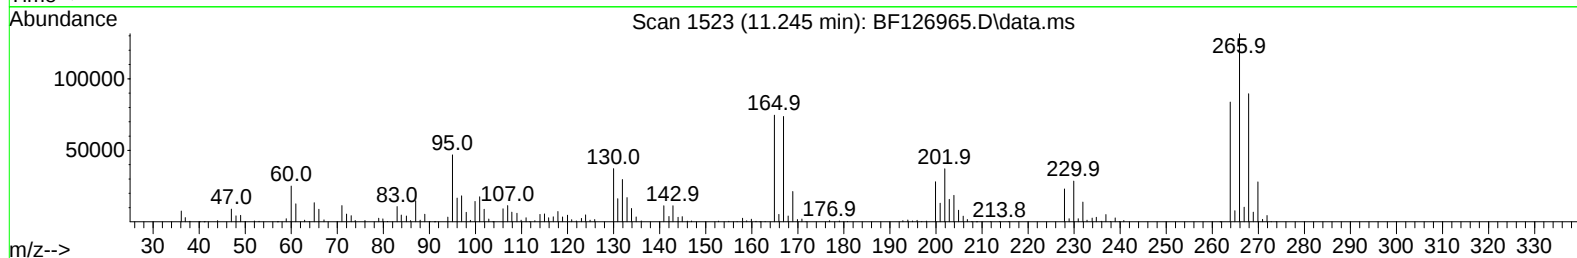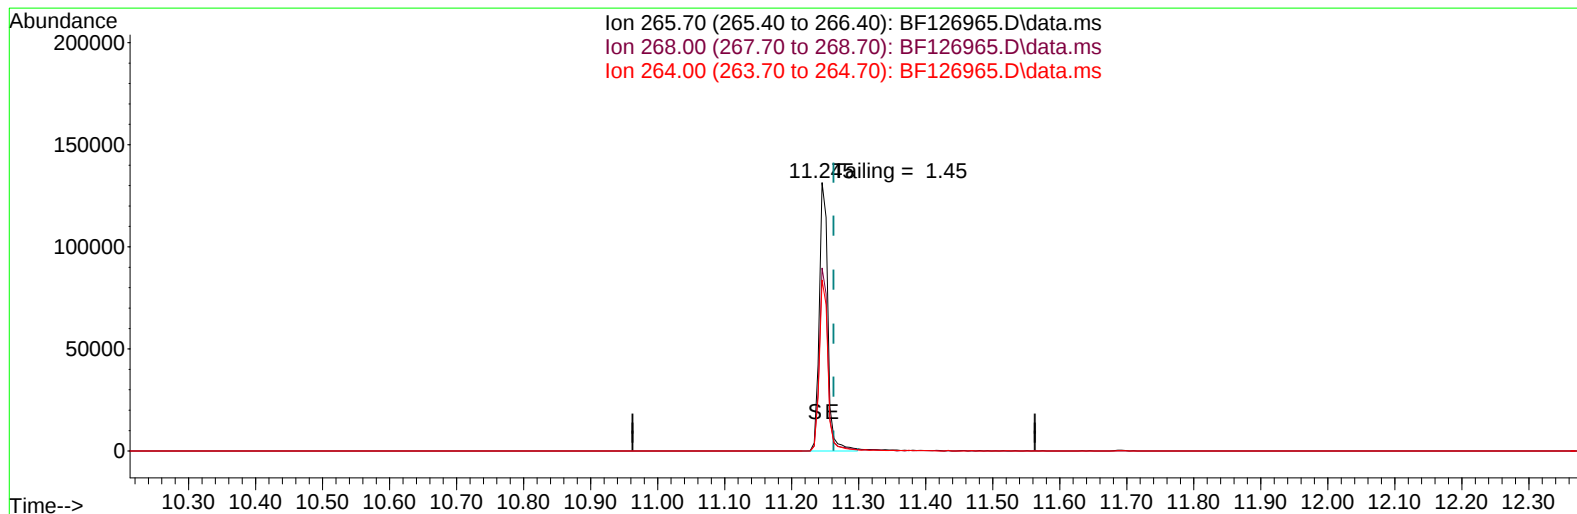

TIC: BF126965.D\data.ms

(70) Pentachlorophenol (C)

11.245min (-0.017) 22890.87 ng




response 119940

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	68.15
264.00	63.00	63.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022122\
 Data File : BF126965.D
 Acq On : 21 Feb 2022 10:59
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 21 13:12:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 16 14:55:48 2022
 Response via : Initial Calibration

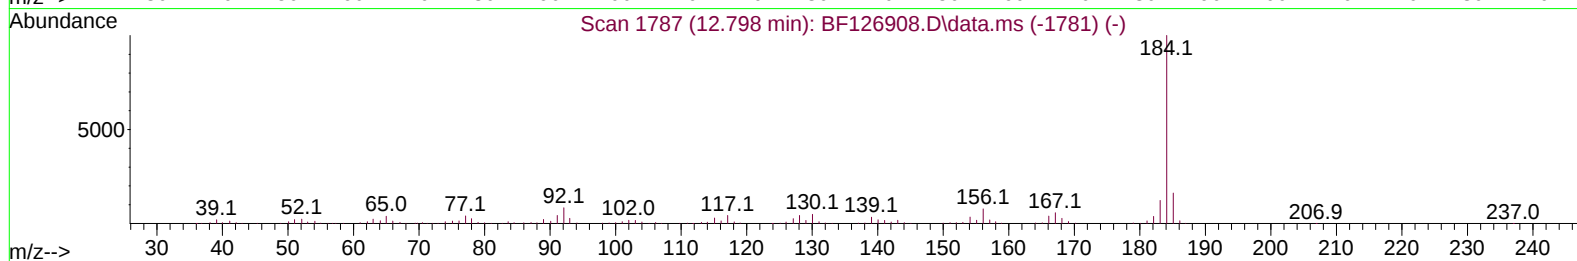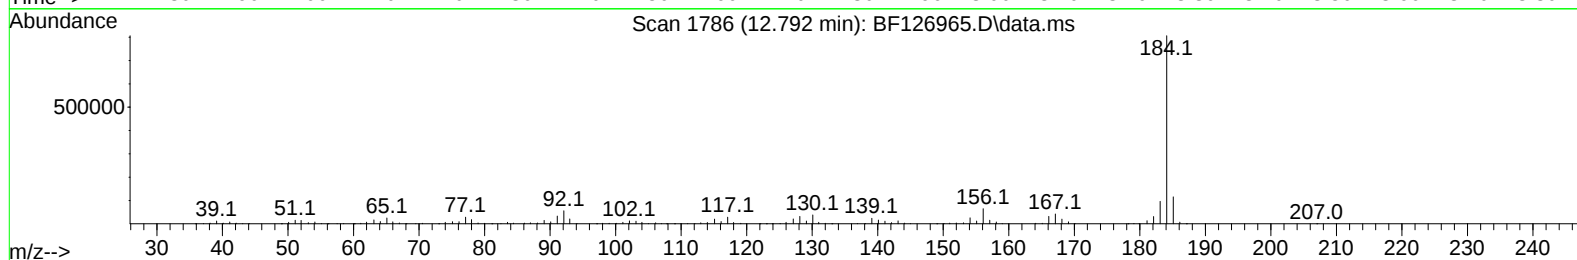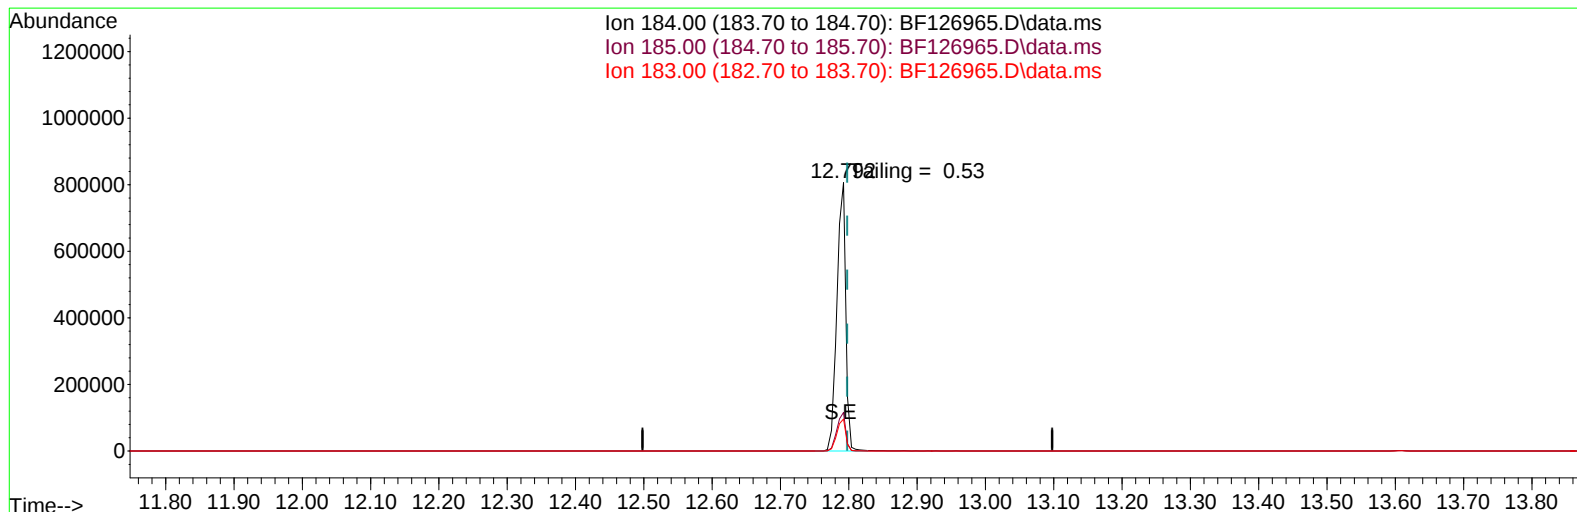

TIC: BF126965.D\data.ms

(77) Benzidine

12.792min (-0.006) 0.00 ng

response 728671

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.35
183.00	10.20	11.96
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/21/2022	BNA_F	<u>BF126965.D</u>
Compound Name	Response	Retention Time
DDT	330618	13.61
DDD	299	13.3
DDE	95	12.96
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
394	331012	0.12

Instrument :
BNA_F
ClientSampleId :
DFTPP