
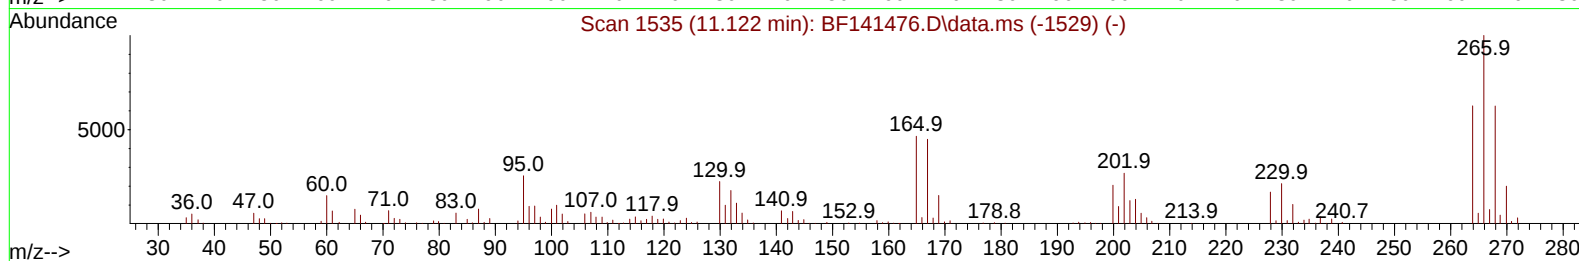
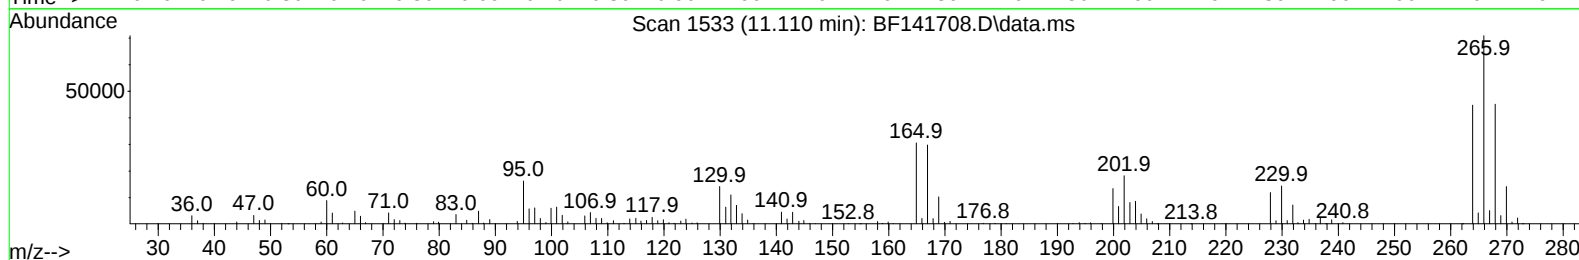


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022125\
Data File : BF141708.D
Acq On : 21 Feb 2025 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 10:34:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

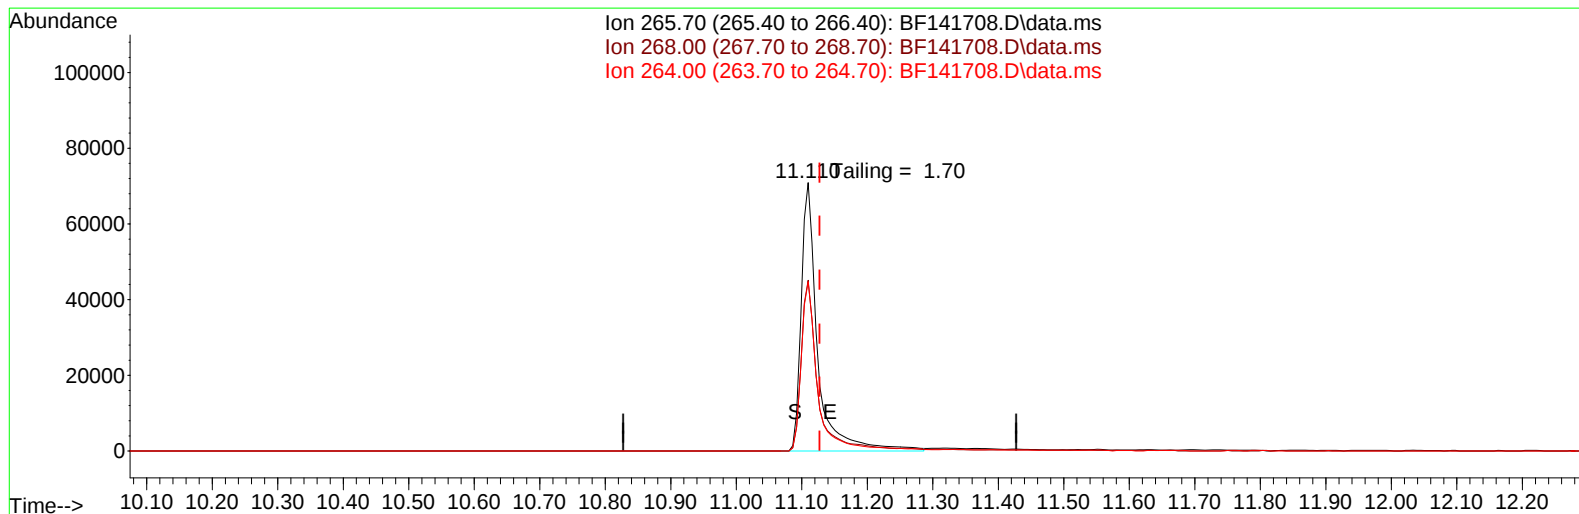

TIC: BF141708.D\data.ms

(70) Pentachlorophenol (C)




11.110min (-0.018) 29209.87 ng

response 124456

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.65
264.00	62.60	63.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022125\
Data File : BF141708.D
Acq On : 21 Feb 2025 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 10:34:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

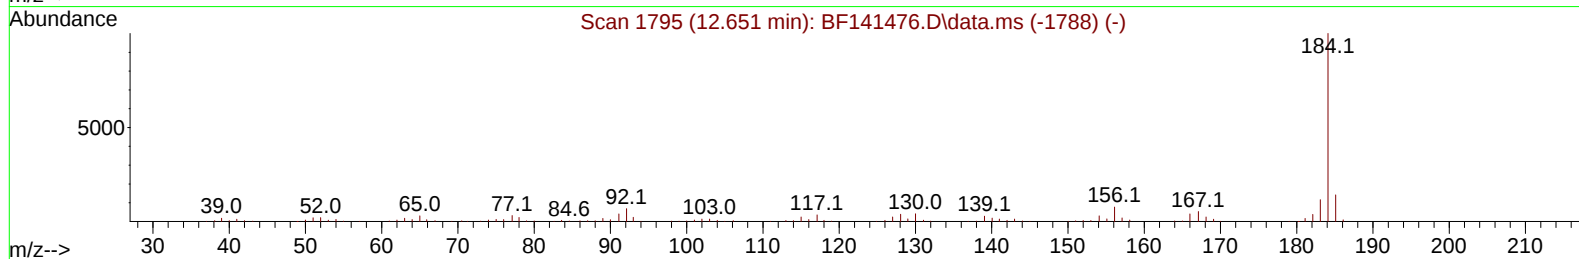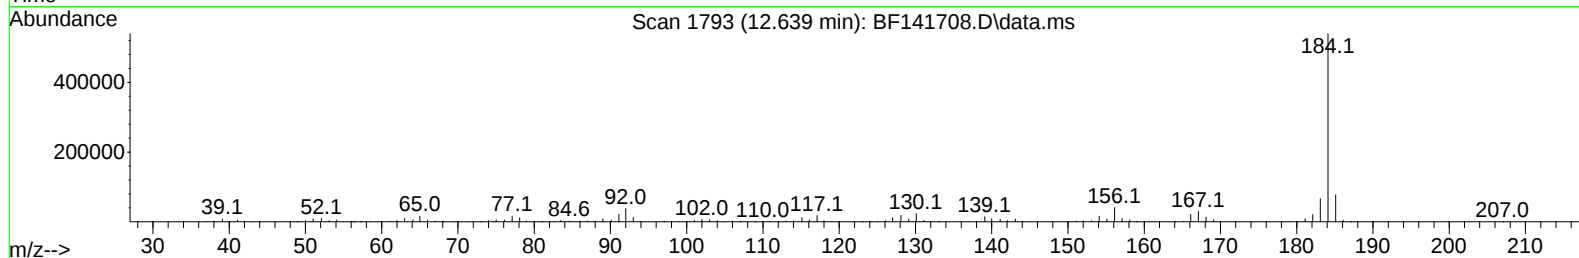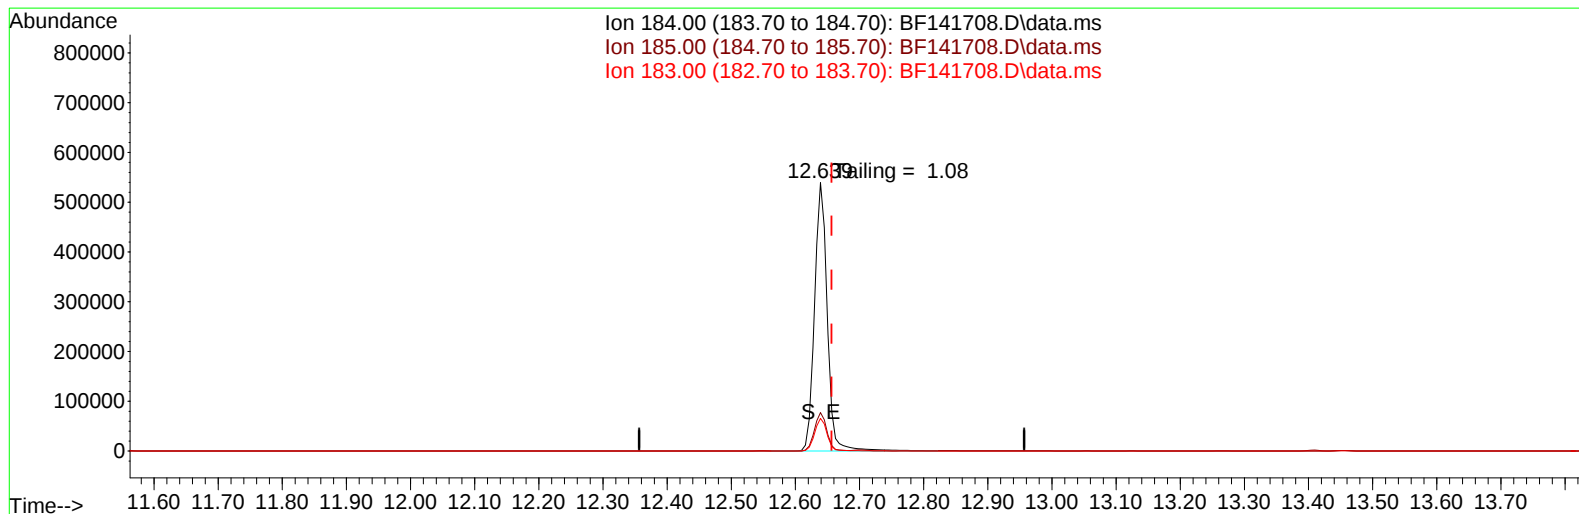

TIC: BF141708.D\data.ms

(77) Benzidine

12.639min (-0.018) 0.00 ng

response 747800

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.31
183.00	11.60	12.19
0.00	0.00	0.00