

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022125\
 Data File : BF141710.D
 Acq On : 21 Feb 2025 10:15
 Operator : RC/JU
 Sample : PB166801BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB166801BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141710.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.410	558	564	591	rBV	2122281	2920895	81.64%	13.902%
2	6.422	730	736	756	rBV	2031340	2925252	81.76%	13.923%
3	6.775	791	796	812	rVB	454310	600499	16.78%	2.858%
4	7.345	886	893	927	rBV	1353372	1967754	55.00%	9.366%
5	8.063	1009	1015	1034	rBV	536878	791133	22.11%	3.766%
6	9.133	1191	1197	1217	rBV	2604143	3577991	100.00%	17.030%
7	9.810	1307	1312	1337	rVB	634364	885815	24.76%	4.216%
8	10.604	1441	1447	1479	rBV	1425203	1997660	55.83%	9.508%
9	11.298	1559	1565	1580	rBV	615477	863476	24.13%	4.110%
10	12.880	1828	1834	1846	rBV	2425258	3373662	94.29%	16.057%
11	13.933	2008	2013	2025	rBV	414538	598314	16.72%	2.848%
12	15.380	2252	2259	2275	rBV	256646	469708	13.13%	2.236%
13	16.298	2410	2415	2431	rVB2	12797	37840	1.06%	0.180%




Sum of corrected areas: 21009999

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022125\
Data File : BF141710.D
Acq On : 21 Feb 2025 10:15
Operator : RC/JU
Sample : PB166801BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166801BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

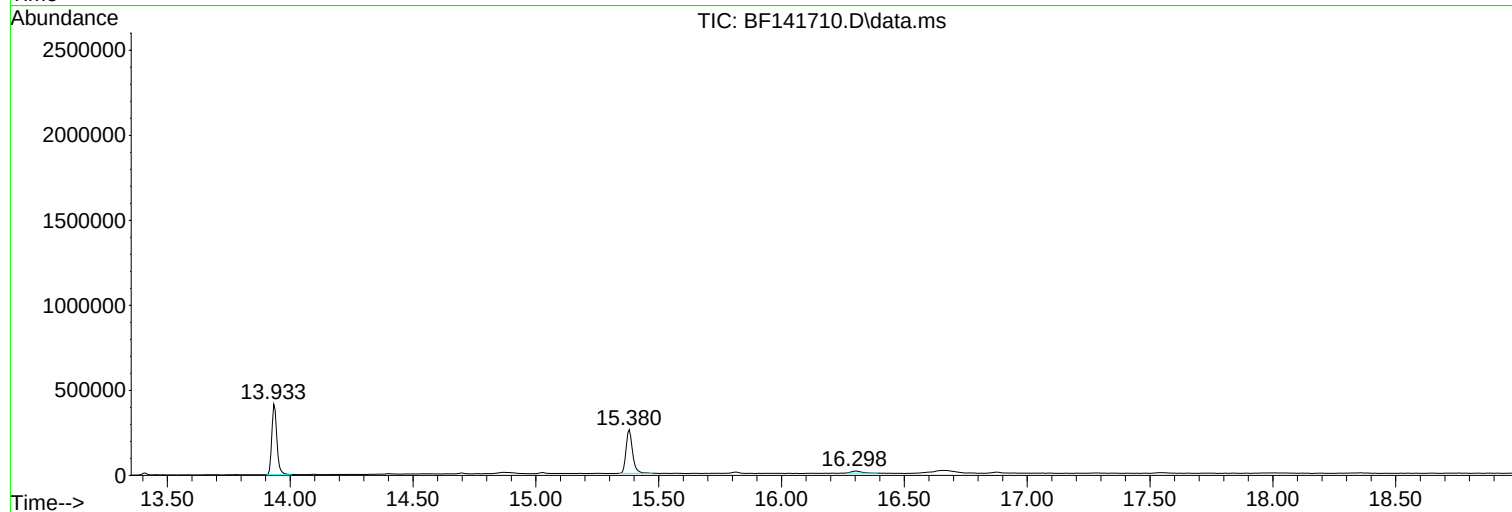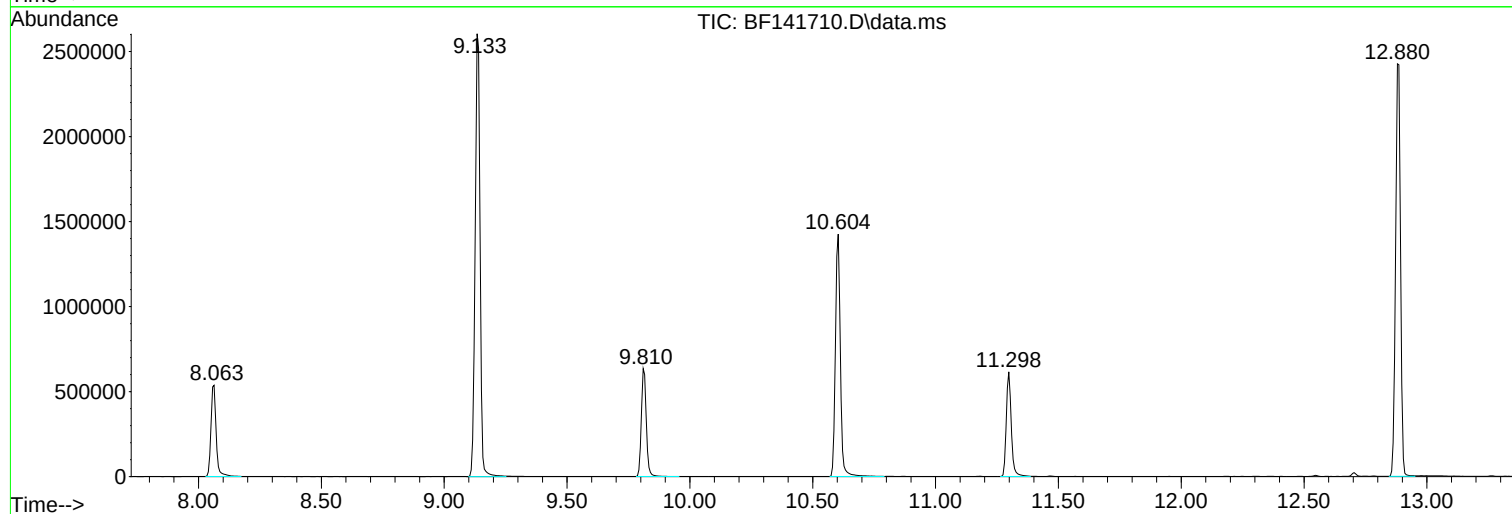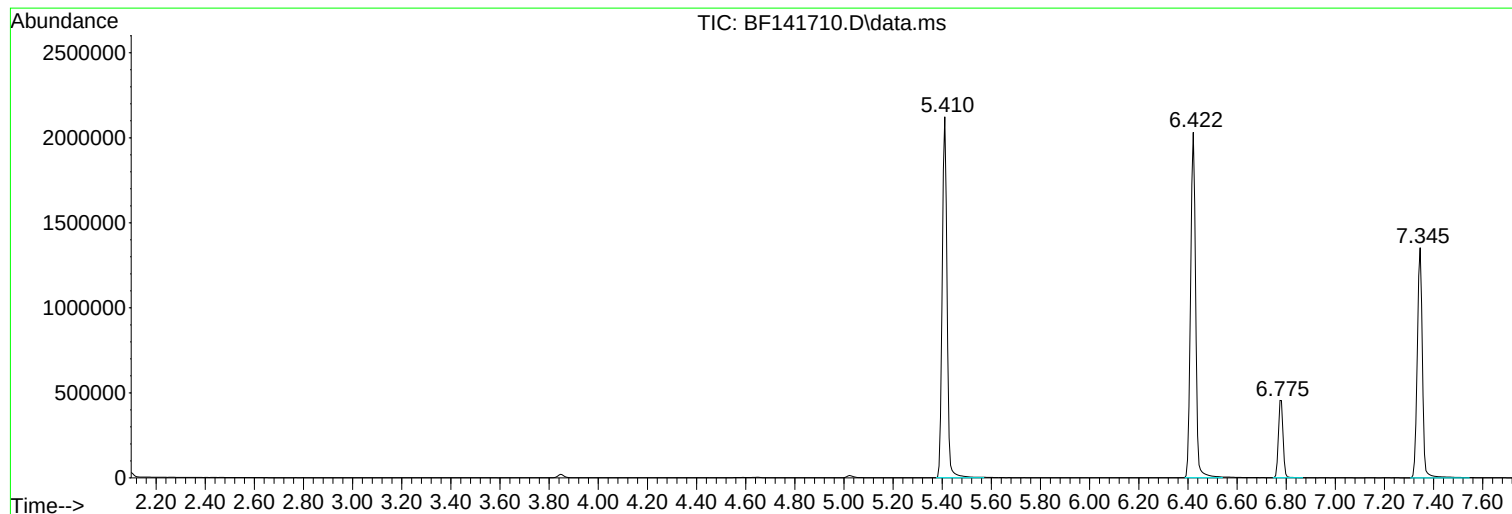

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022125\
Data File : BF141710.D
Acq On : 21 Feb 2025 10:15
Operator : RC/JU
Sample : PB166801BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166801BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022125\
Data File : BF141710.D
Acq On : 21 Feb 2025 10:15
Operator : RC/JU
Sample : PB166801BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166801BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------