

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022125\
Data File : BF141713.D
Acq On : 21 Feb 2025 11:44
Operator : RC/JU
Sample : PB166806BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166806BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141713.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.410	558	564	599	rBV	2070839	2881784	81.75%	14.127%
2	6.422	730	736	775	rBV	1987191	2894959	82.12%	14.191%
3	6.781	791	797	810	rVB	428100	563385	15.98%	2.762%
4	7.345	886	893	920	rBV	1335592	1931213	54.78%	9.467%
5	8.063	1009	1015	1033	rBV	500903	742776	21.07%	3.641%
6	9.133	1191	1197	1218	rBV	2588096	3525306	100.00%	17.281%
7	9.810	1307	1312	1336	rBV	598385	835684	23.71%	4.097%
8	10.604	1441	1447	1480	rBV	1386070	1956638	55.50%	9.592%
9	11.298	1559	1565	1590	rBV	567537	813617	23.08%	3.988%
10	12.880	1828	1834	1853	rBV	2461428	3276442	92.94%	16.062%
11	13.933	2008	2013	2026	rBV	355352	540081	15.32%	2.648%
12	15.380	2252	2259	2276	rBV	233021	437441	12.41%	2.144%




Sum of corrected areas: 20399326

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022125\
Data File : BF141713.D
Acq On : 21 Feb 2025 11:44
Operator : RC/JU
Sample : PB166806BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166806BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

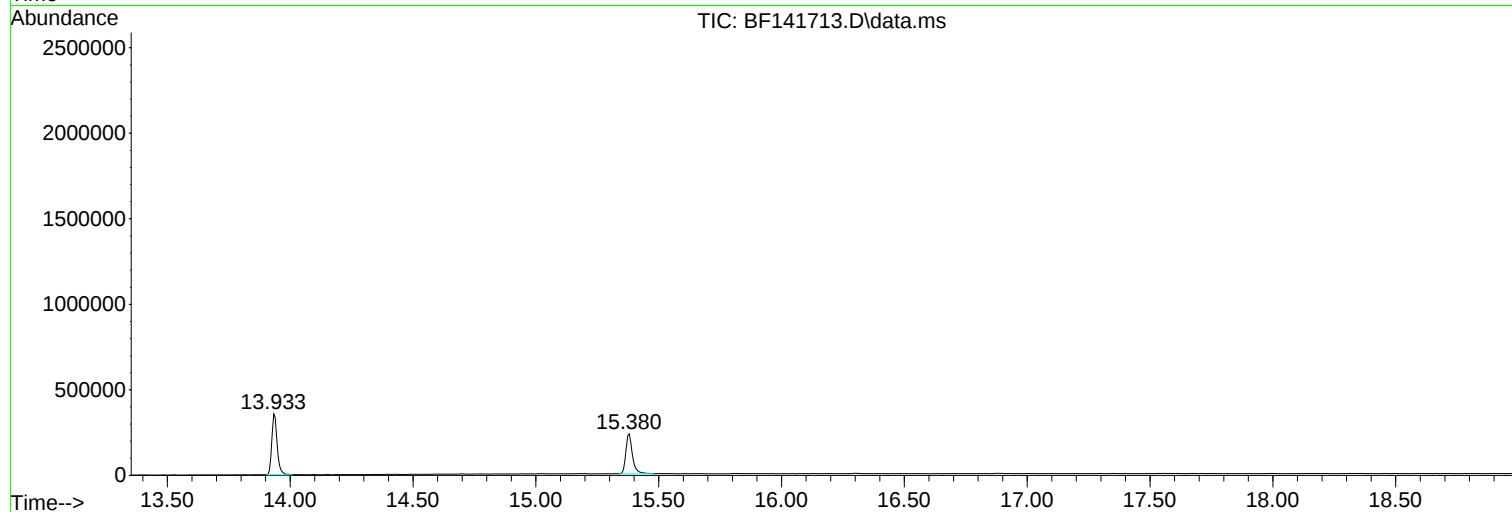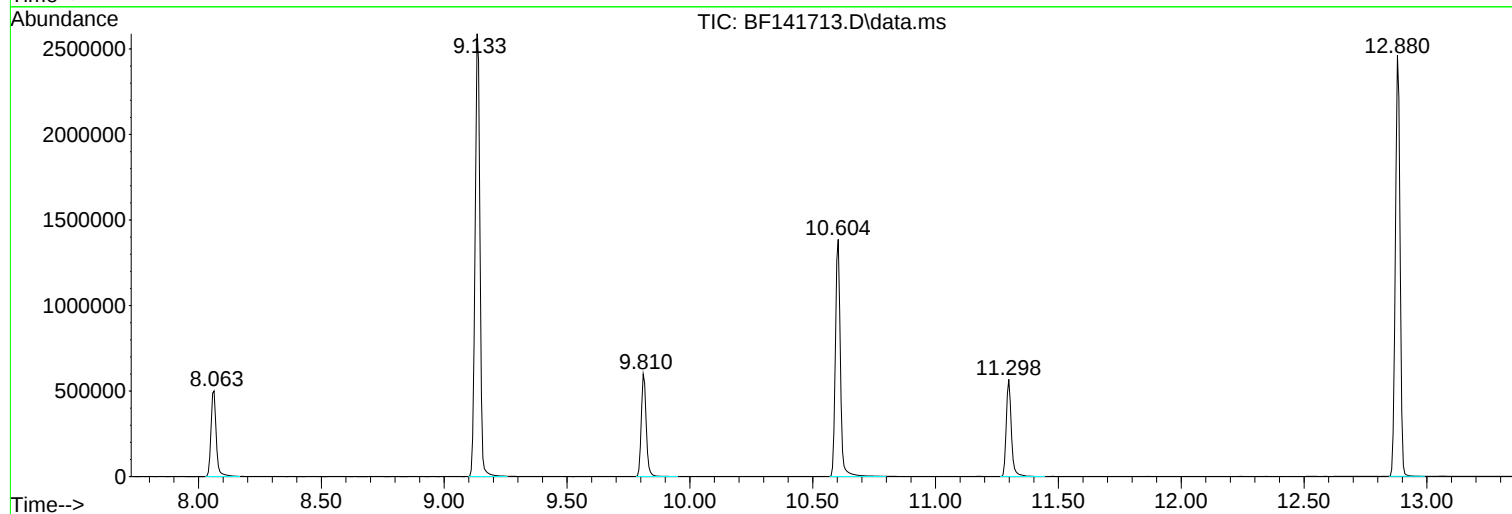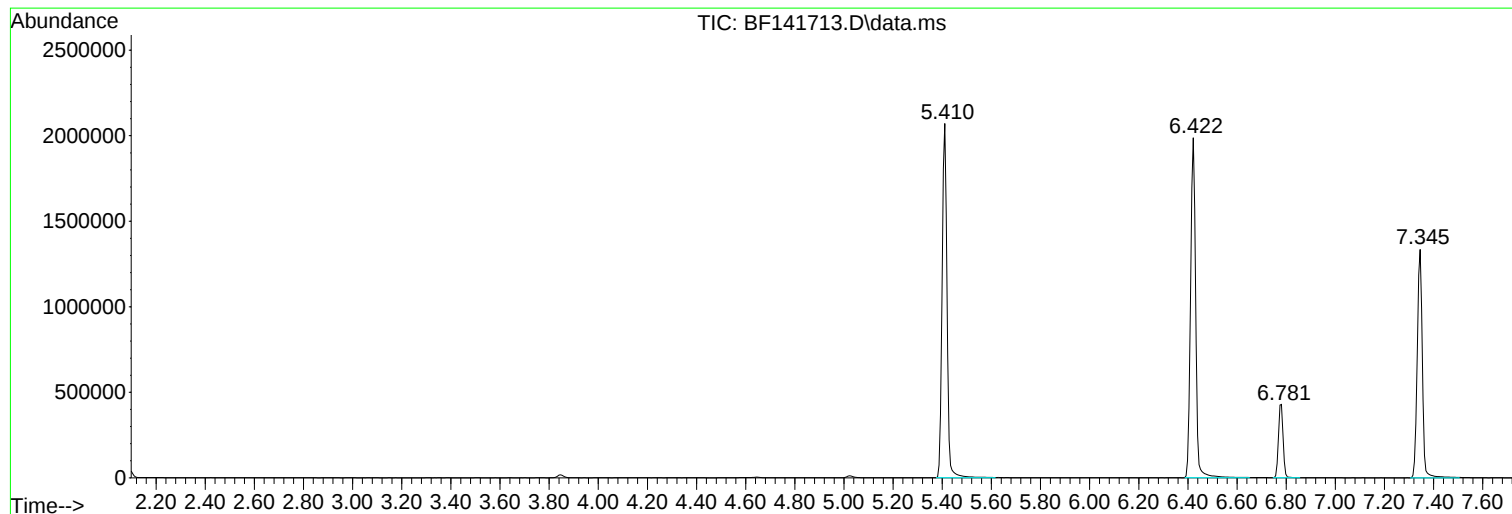

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022125\
Data File : BF141713.D
Acq On : 21 Feb 2025 11:44
Operator : RC/JU
Sample : PB166806BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166806BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022125\
Data File : BF141713.D
Acq On : 21 Feb 2025 11:44
Operator : RC/JU
Sample : PB166806BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166806BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------