

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022125\
Data File : BF141715.D
Acq On : 21 Feb 2025 12:44
Operator : RC/JU
Sample : PB166796BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166796BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141715.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.410	558	564	601	rBV	2086455	2895586	82.11%	14.179%
2	6.422	730	736	766	rBV	2006517	2910937	82.54%	14.254%
3	6.781	791	797	807	rBV	427740	556228	15.77%	2.724%
4	7.345	886	893	922	rBV	1356394	1945610	55.17%	9.527%
5	8.063	1009	1015	1041	rBV	500141	731364	20.74%	3.581%
6	9.133	1191	1197	1225	rBV	2556506	3526666	100.00%	17.269%
7	9.816	1307	1313	1329	rBV	562585	812903	23.05%	3.980%
8	10.604	1441	1447	1472	rBV	1395954	1955802	55.46%	9.577%
9	11.298	1560	1565	1586	rBV	560838	801393	22.72%	3.924%
10	12.886	1828	1835	1846	rBV	2424427	3326431	94.32%	16.288%
11	13.939	2008	2014	2029	rBV	356214	537850	15.25%	2.634%
12	15.380	2253	2259	2280	rVB	229671	421383	11.95%	2.063%




Sum of corrected areas: 20422153

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022125\
Data File : BF141715.D
Acq On : 21 Feb 2025 12:44
Operator : RC/JU
Sample : PB166796BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166796BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

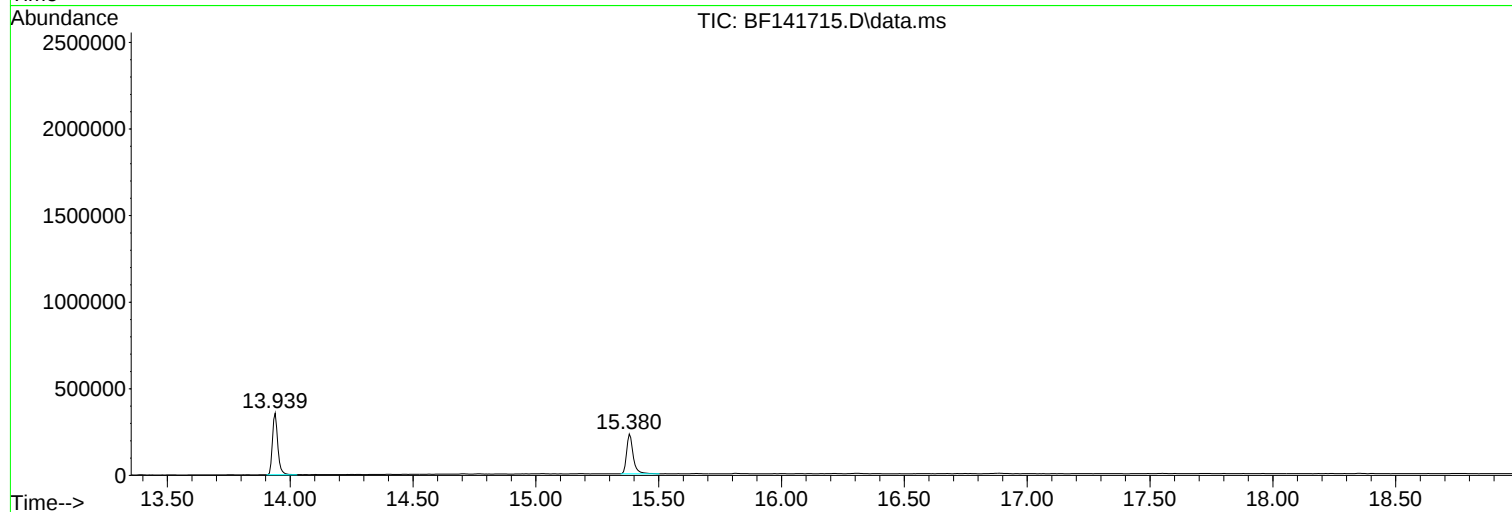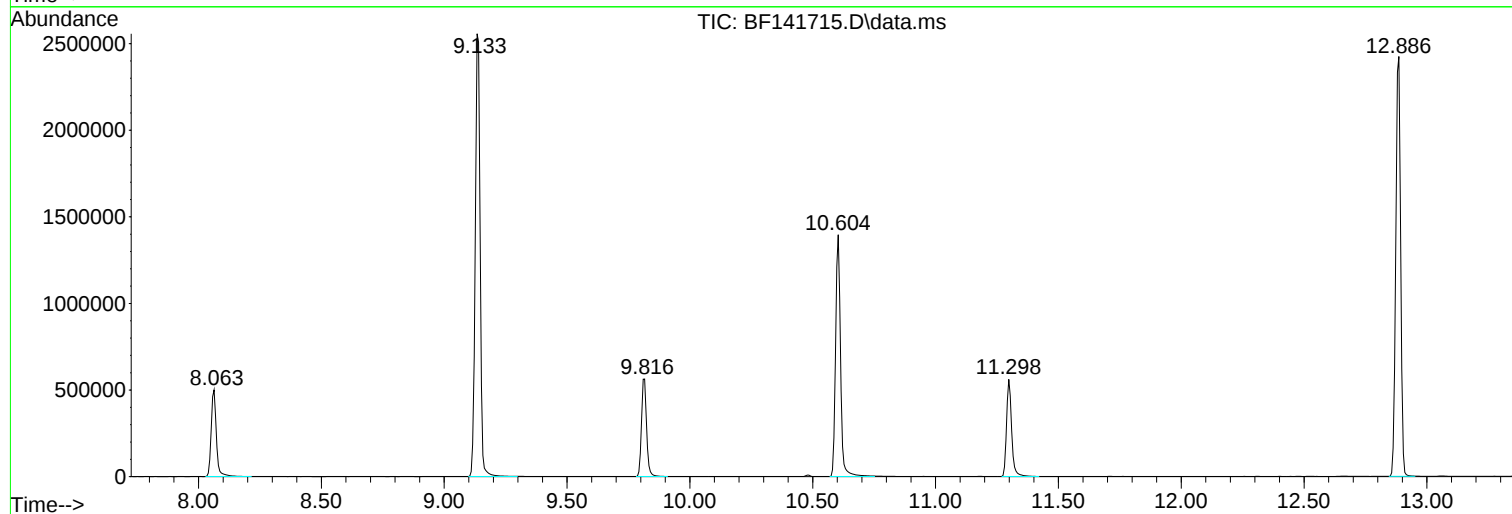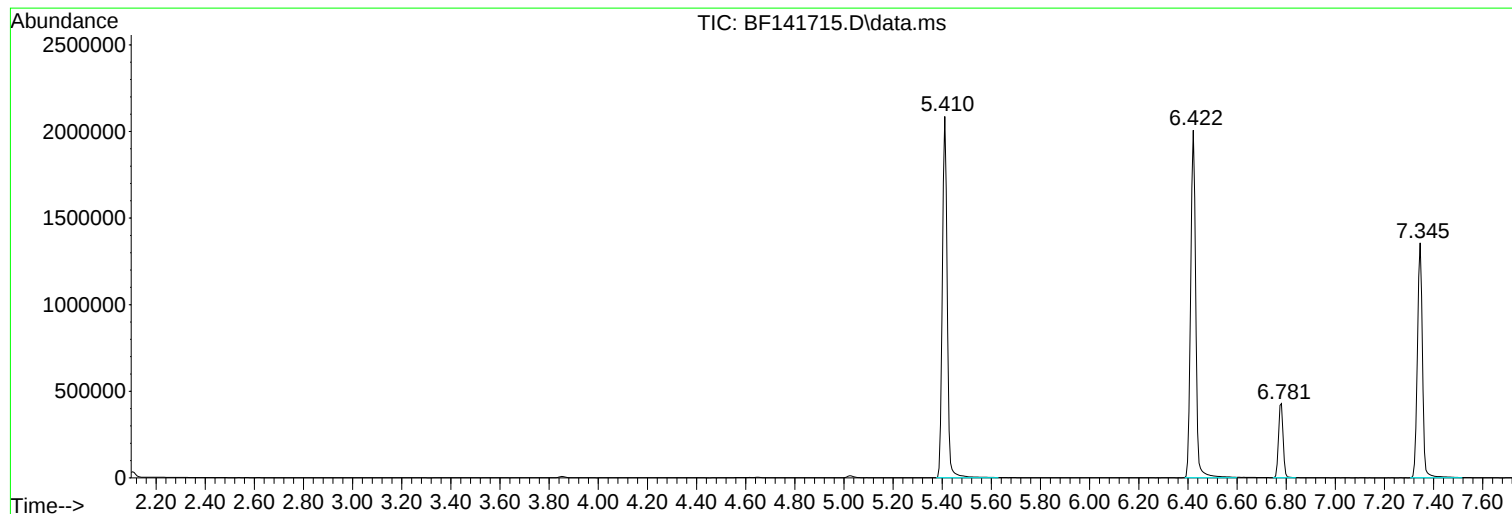

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022125\
Data File : BF141715.D
Acq On : 21 Feb 2025 12:44
Operator : RC/JU
Sample : PB166796BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166796BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022125\
Data File : BF141715.D
Acq On : 21 Feb 2025 12:44
Operator : RC/JU
Sample : PB166796BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166796BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------