
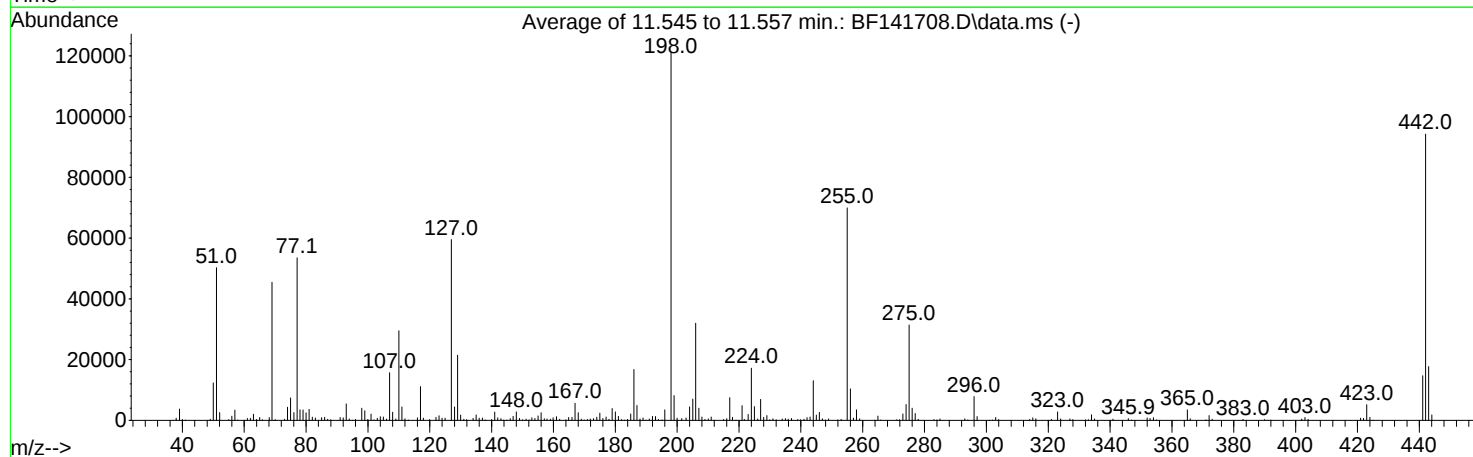


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022125\
Data File : BF141708.D
Acq On : 21 Feb 2025 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 06 16:58:59 2025

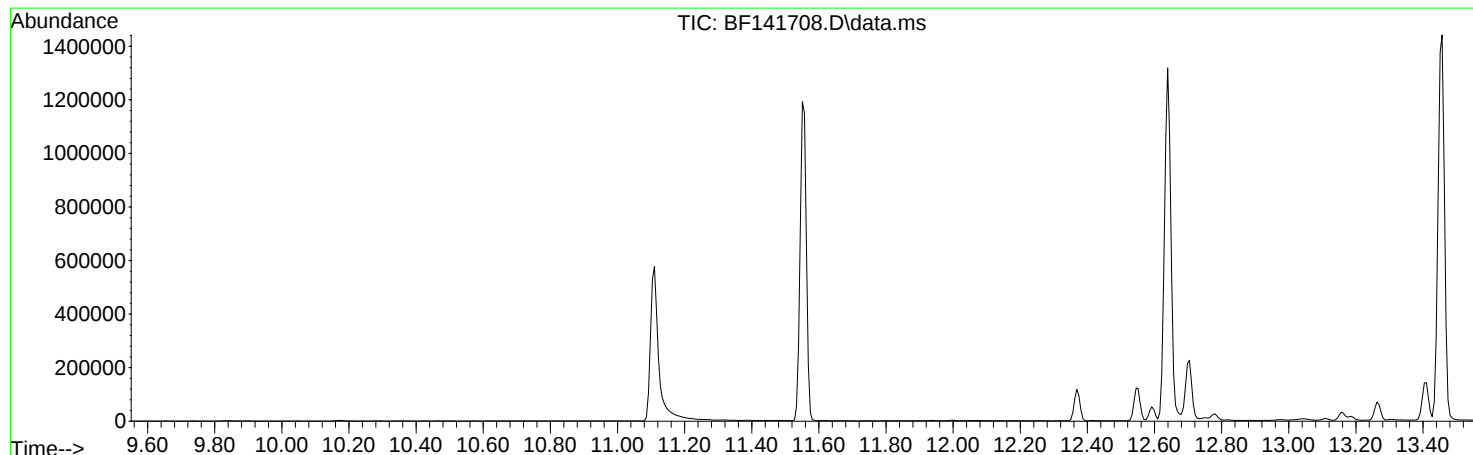

AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	50237	PASS
68	69	0.00	2	2.0	888	PASS
69	198	0.00	100	37.5	45453	PASS
70	69	0.00	2	0.5	246	PASS
127	198	10	80	49.2	59525	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	121101	PASS
199	198	5	9	6.8	8182	PASS
275	198	10	60	25.9	31421	PASS
365	198	1	100	2.9	3498	PASS
441	198	0.01	100	12.1	14711	PASS
442	442	50	100	100.0	94240	PASS
443	442	15	24	18.8	17690	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/21/2025	BNA_F	<u>BF141708.D</u>
Compound Name	Response	Retention Time
DDT	380872	13.457
DDD	14637	13.157
DDE	761	12.821
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15398	396270	3.89

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022125\
Data File : BF141708.D
Acq On : 21 Feb 2025 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 21 10:34:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

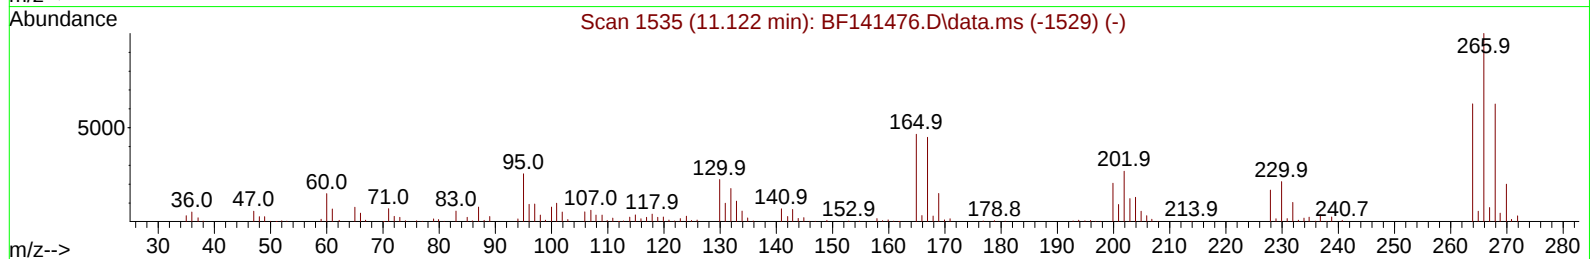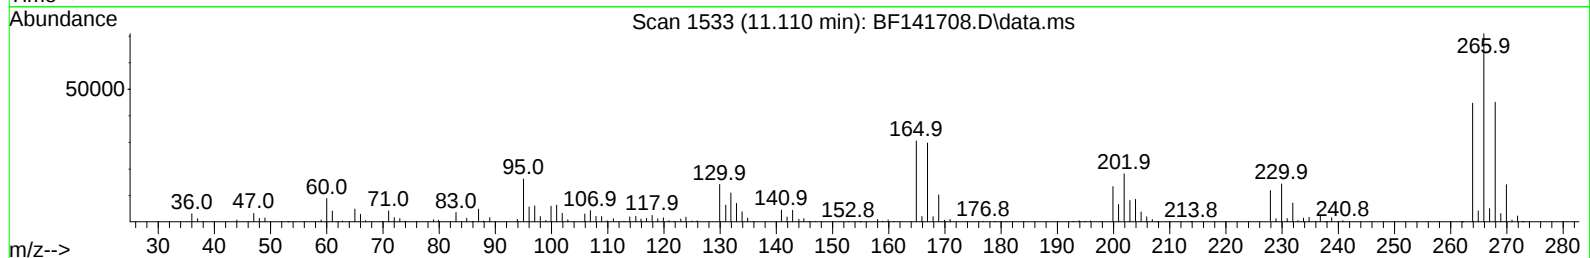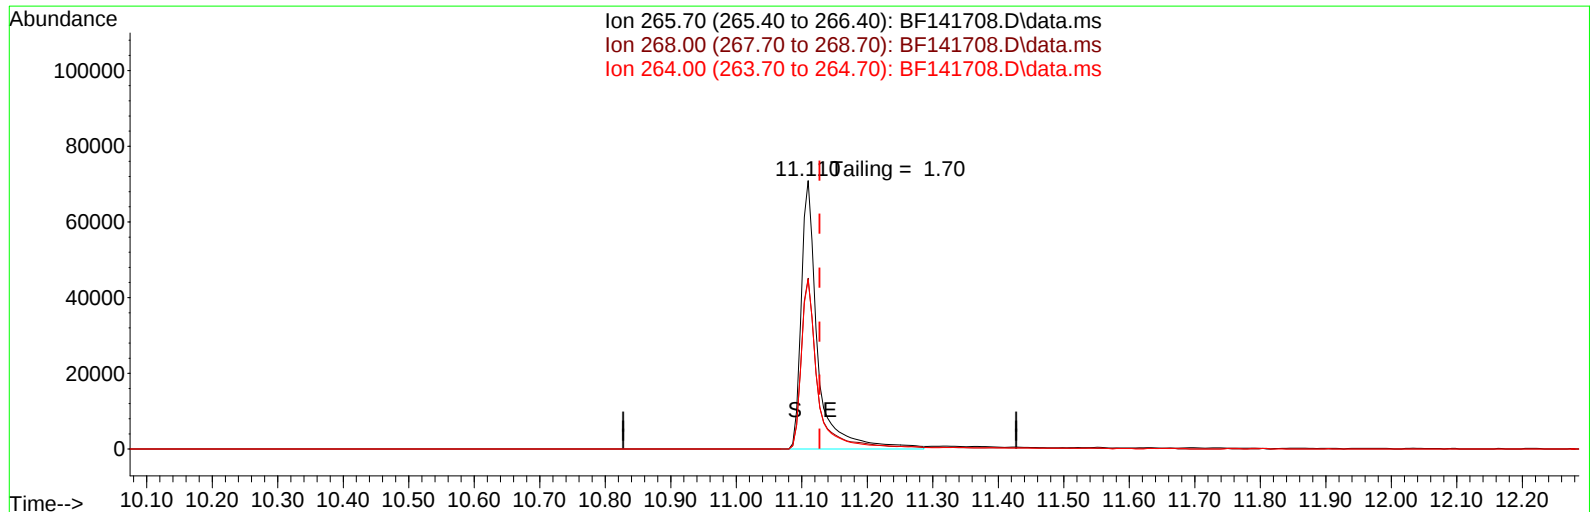

TIC: BF141708.D\data.ms

(70) Pentachlorophenol (C)

11.110min (-0.018) 29209.87 ng




response 124456

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.65
264.00	62.60	63.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022125\
Data File : BF141708.D
Acq On : 21 Feb 2025 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 21 10:34:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

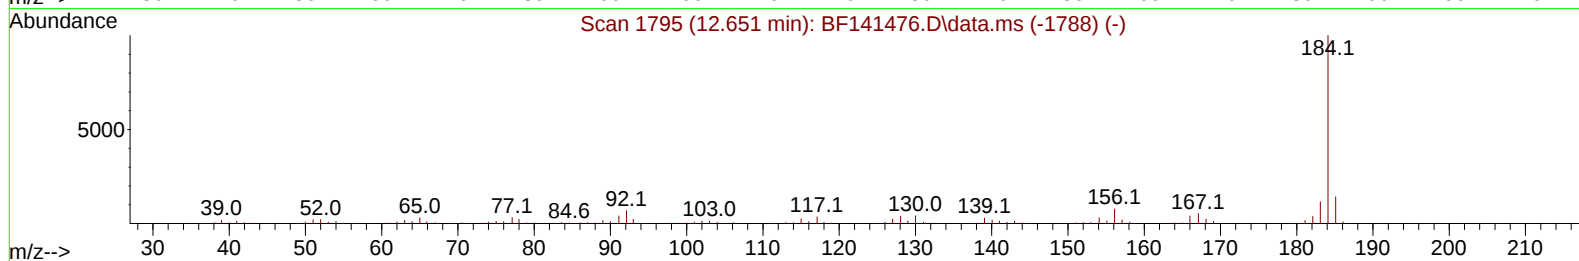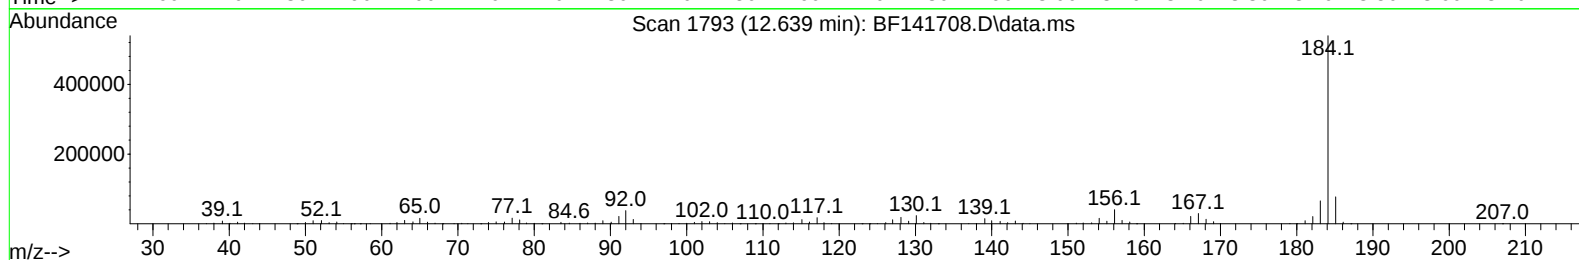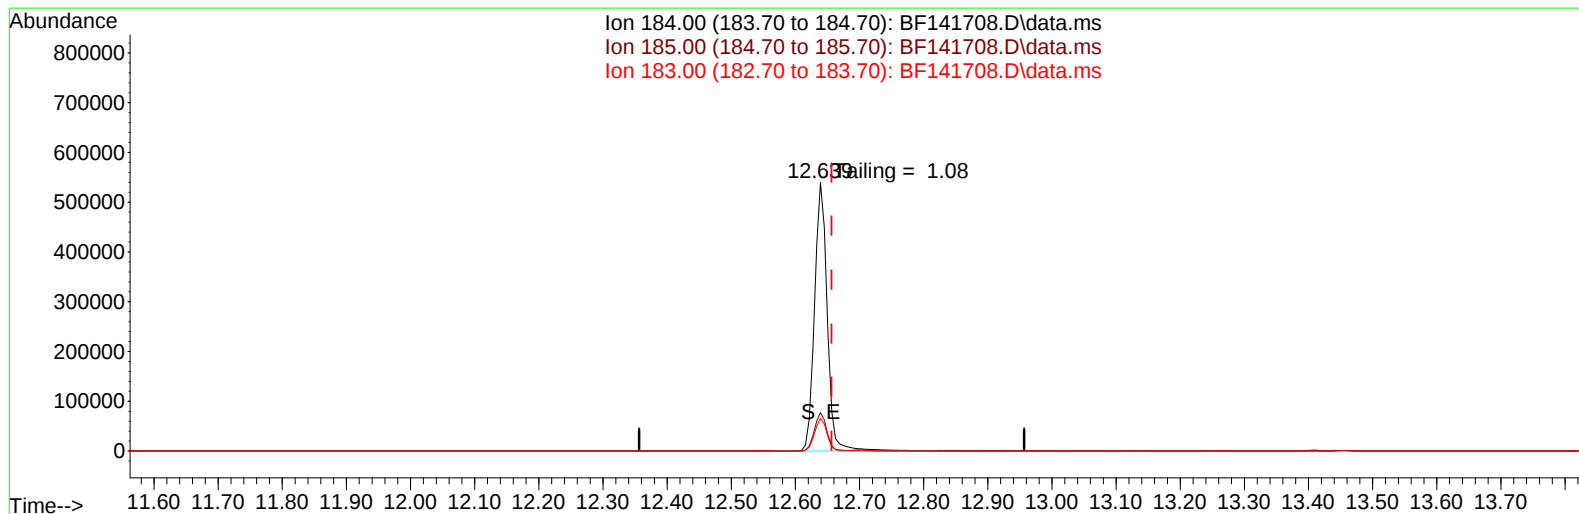

TIC: BF141708.D\data.ms

(77) Benzidine

12.639min (-0.018) 0.00 ng

response 747800

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.31
183.00	11.60	12.19
0.00	0.00	0.00