


Data Path : Z:\HPCHEM1\BNA F\DATA\BF022217\
 Data File : BF093073.D
 Acq On : 22 Feb 2017 14:06
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 17 17:31:55 2017

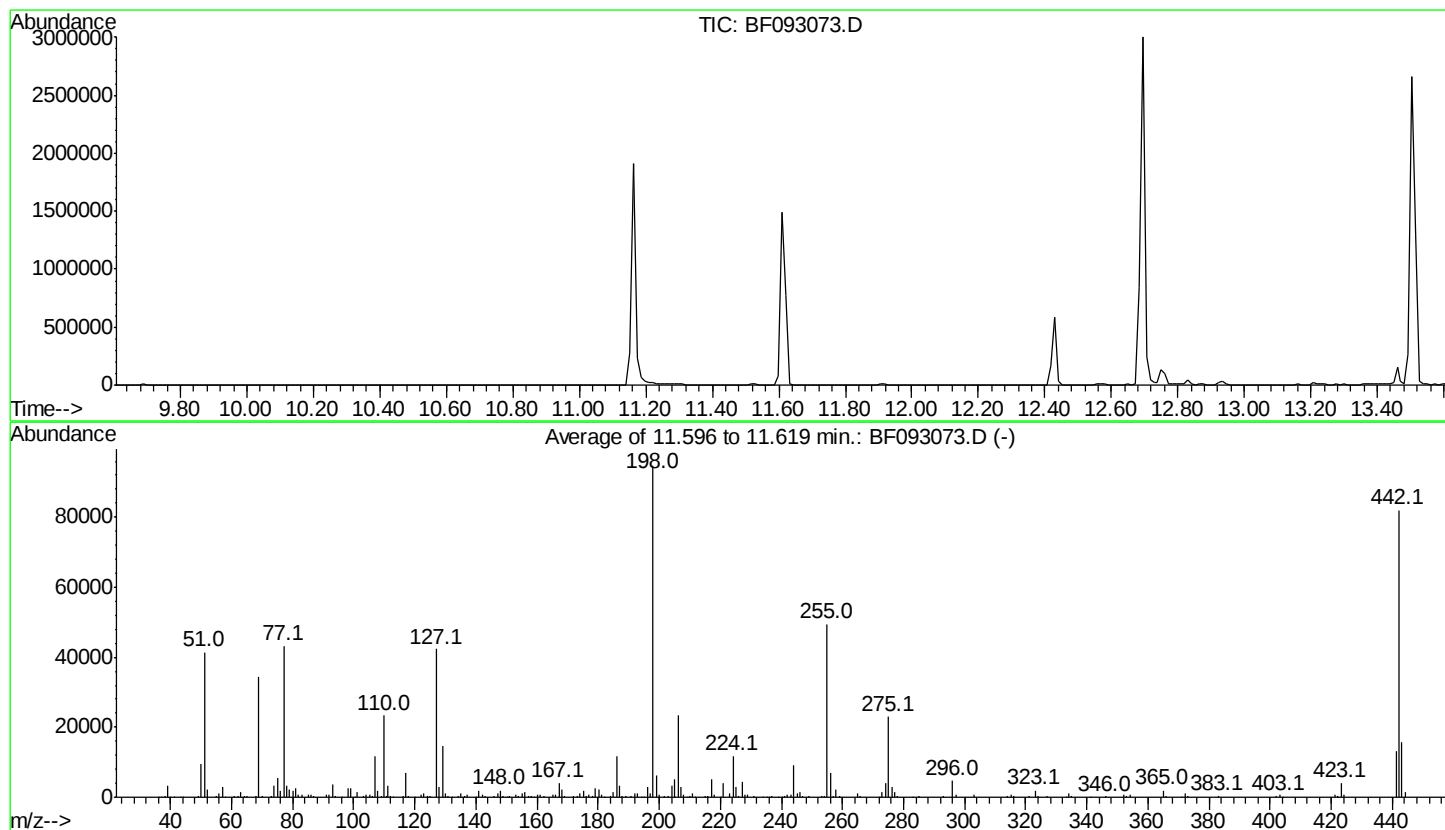

AutoFind: Scans 832, 833, 834; Background Corrected with Scan 829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.7	41442	PASS
68	69	0.00	2	1.5	516	PASS
69	198	0.00	100	36.4	34455	PASS
70	69	0.00	2	0.7	257	PASS
127	198	10	80	44.6	42275	PASS
197	198	0.00	2	1.2	1105	PASS
198	198	100	100	100.0	94728	PASS
199	198	5	9	6.4	6092	PASS
275	198	10	60	24.2	22922	PASS
365	198	1	100	2.1	1951	PASS
441	442	0.01	24	16.1	13213	PASS
442	198	50	100	86.6	82032	PASS
443	442	15	24	19.2	15775	PASS