
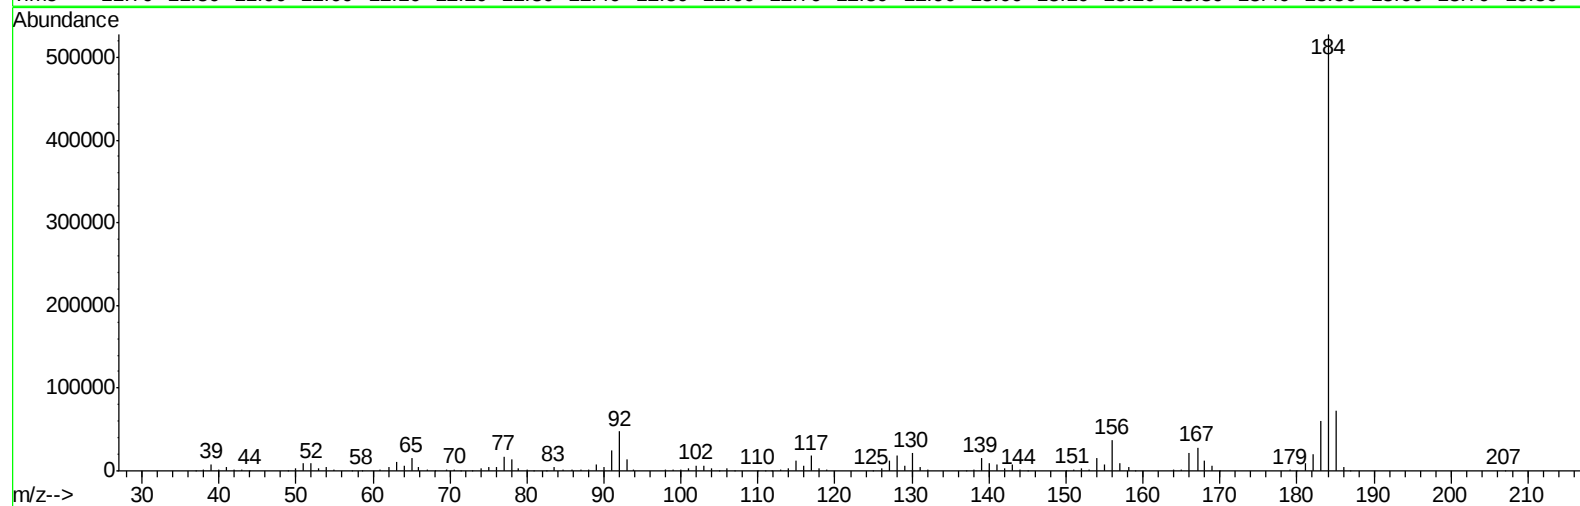


Data Path : Z:\HPCHEM1\BNA F\DATA\BF022218\
Data File : BF103153.D
Acq On : 22 Feb 2018 11:07
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 06:40:18 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 23 02:43:46 2018
Response via : Initial Calibration

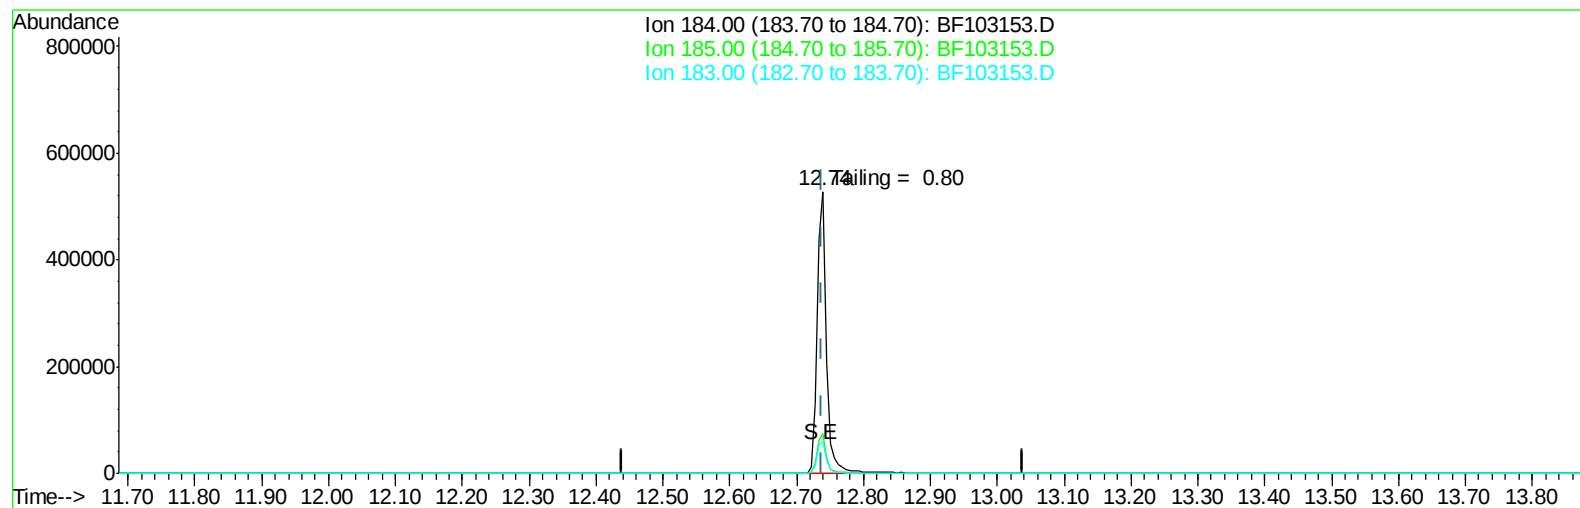

TIC: BF103153.D

(76) Benzidine



12.739min (+0.000) 0.00ng

response 520210

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.90
183.00	11.60	11.48
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF022218\
Data File : BF103153.D
Acq On : 22 Feb 2018 11:07
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 06:40:18 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 23 02:43:46 2018
Response via : Initial Calibration

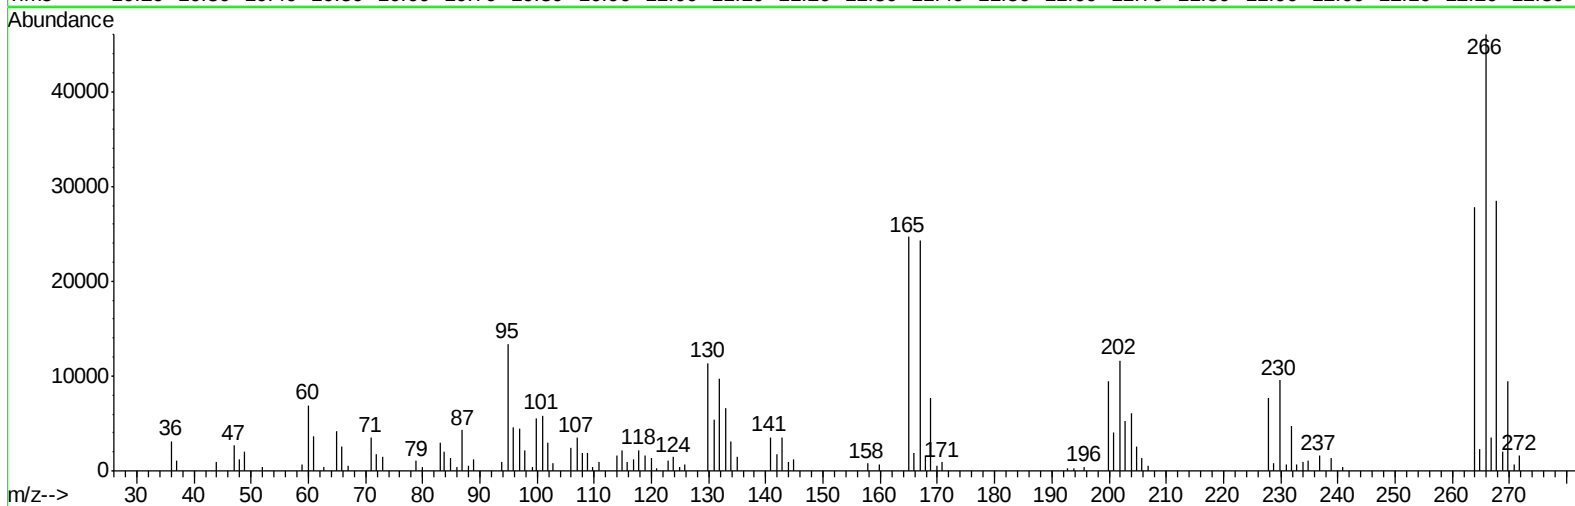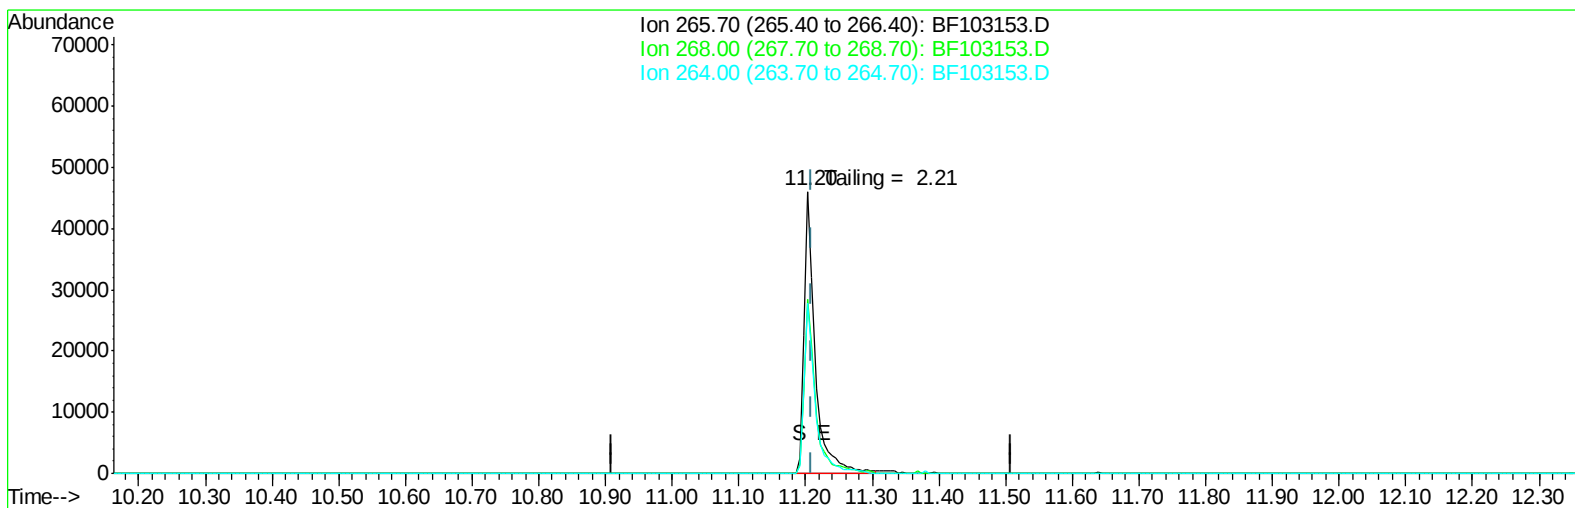

TIC: BF103153.D

(69) Pentachlorophenol (C)

11.204min (-0.006) 73454.60ng

response 52606

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.97
264.00	61.90	60.30
0.00	0.00	0.00