



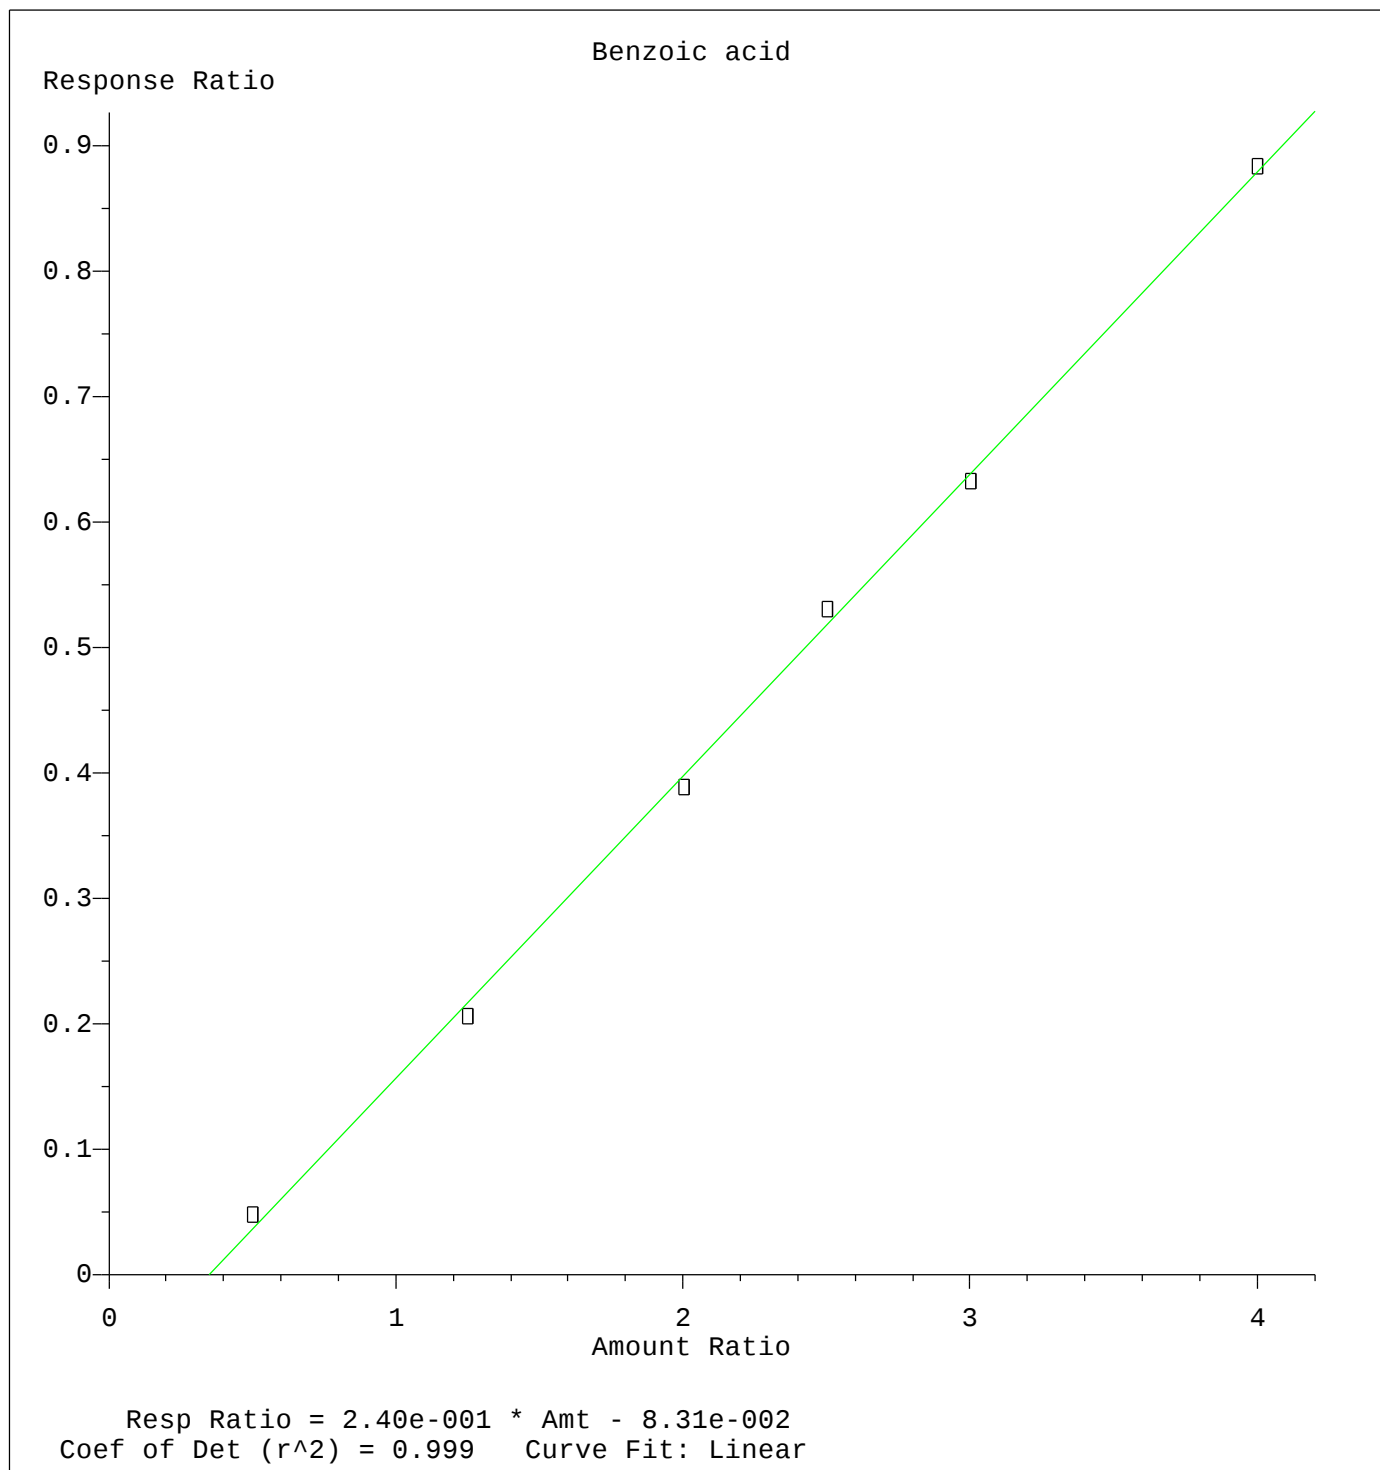

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
Calibration Table Last Updated: Fri Feb 23 02:43:46 2018


Hexachlorocyclopentadiene

Response Ratio

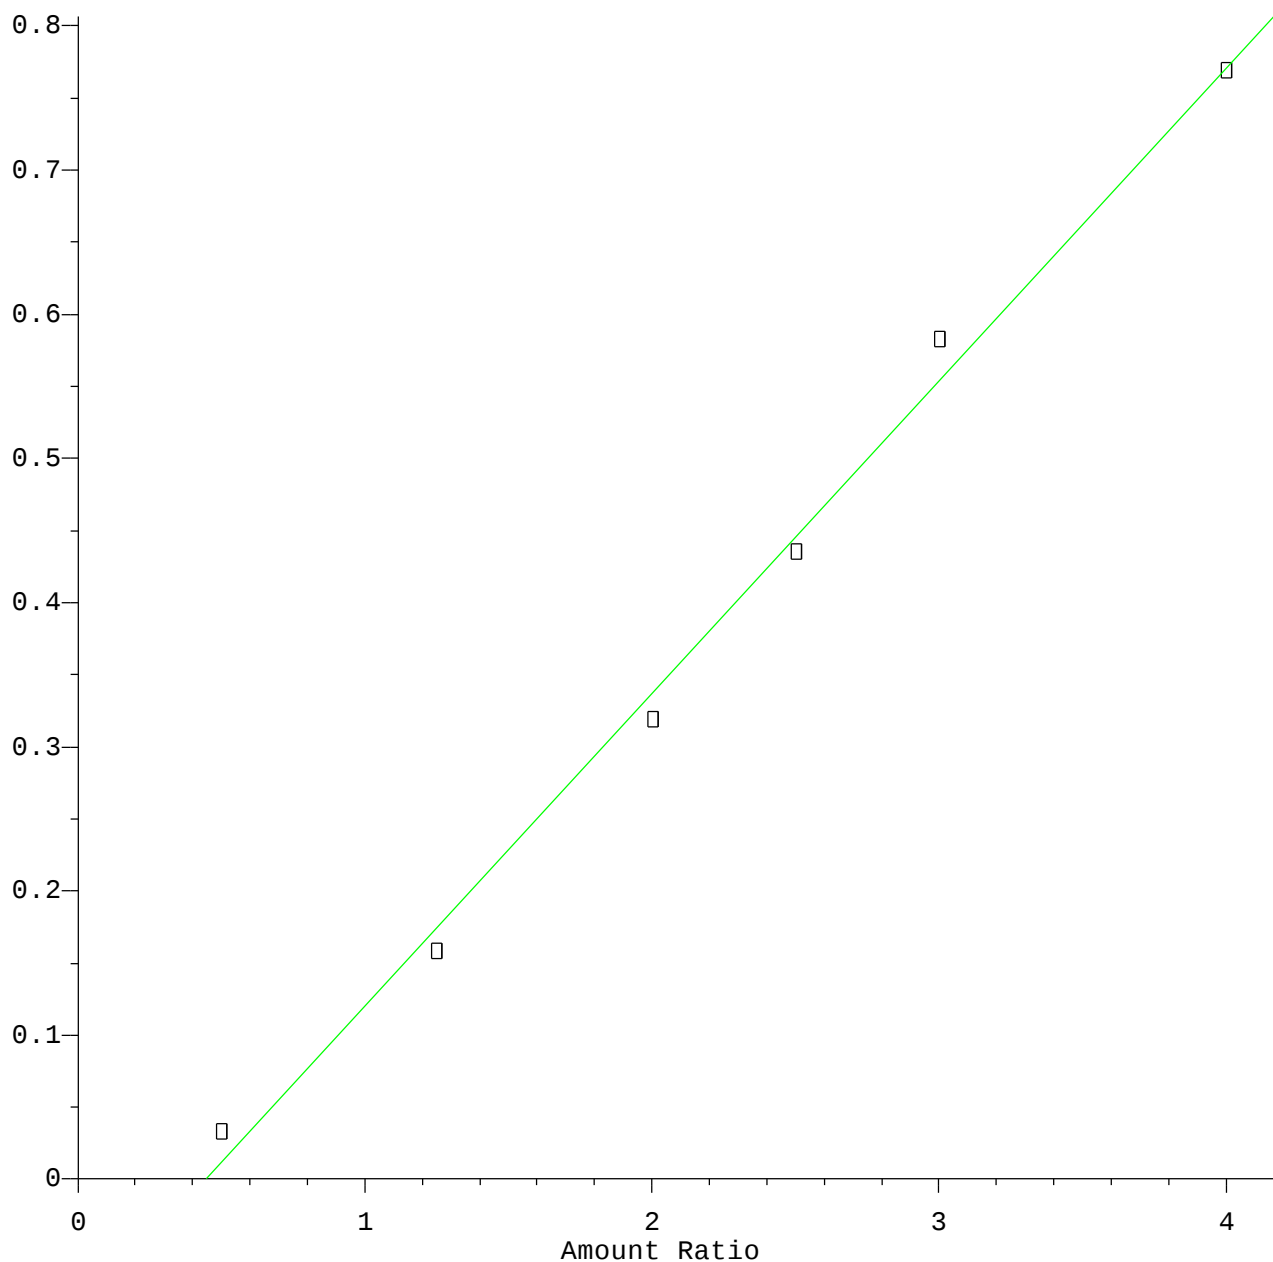


Resp Ratio = $2.17 \times 10^{-1} \times \text{Amt} - 9.63 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
Calibration Table Last Updated: Fri Feb 23 02:43:46 2018

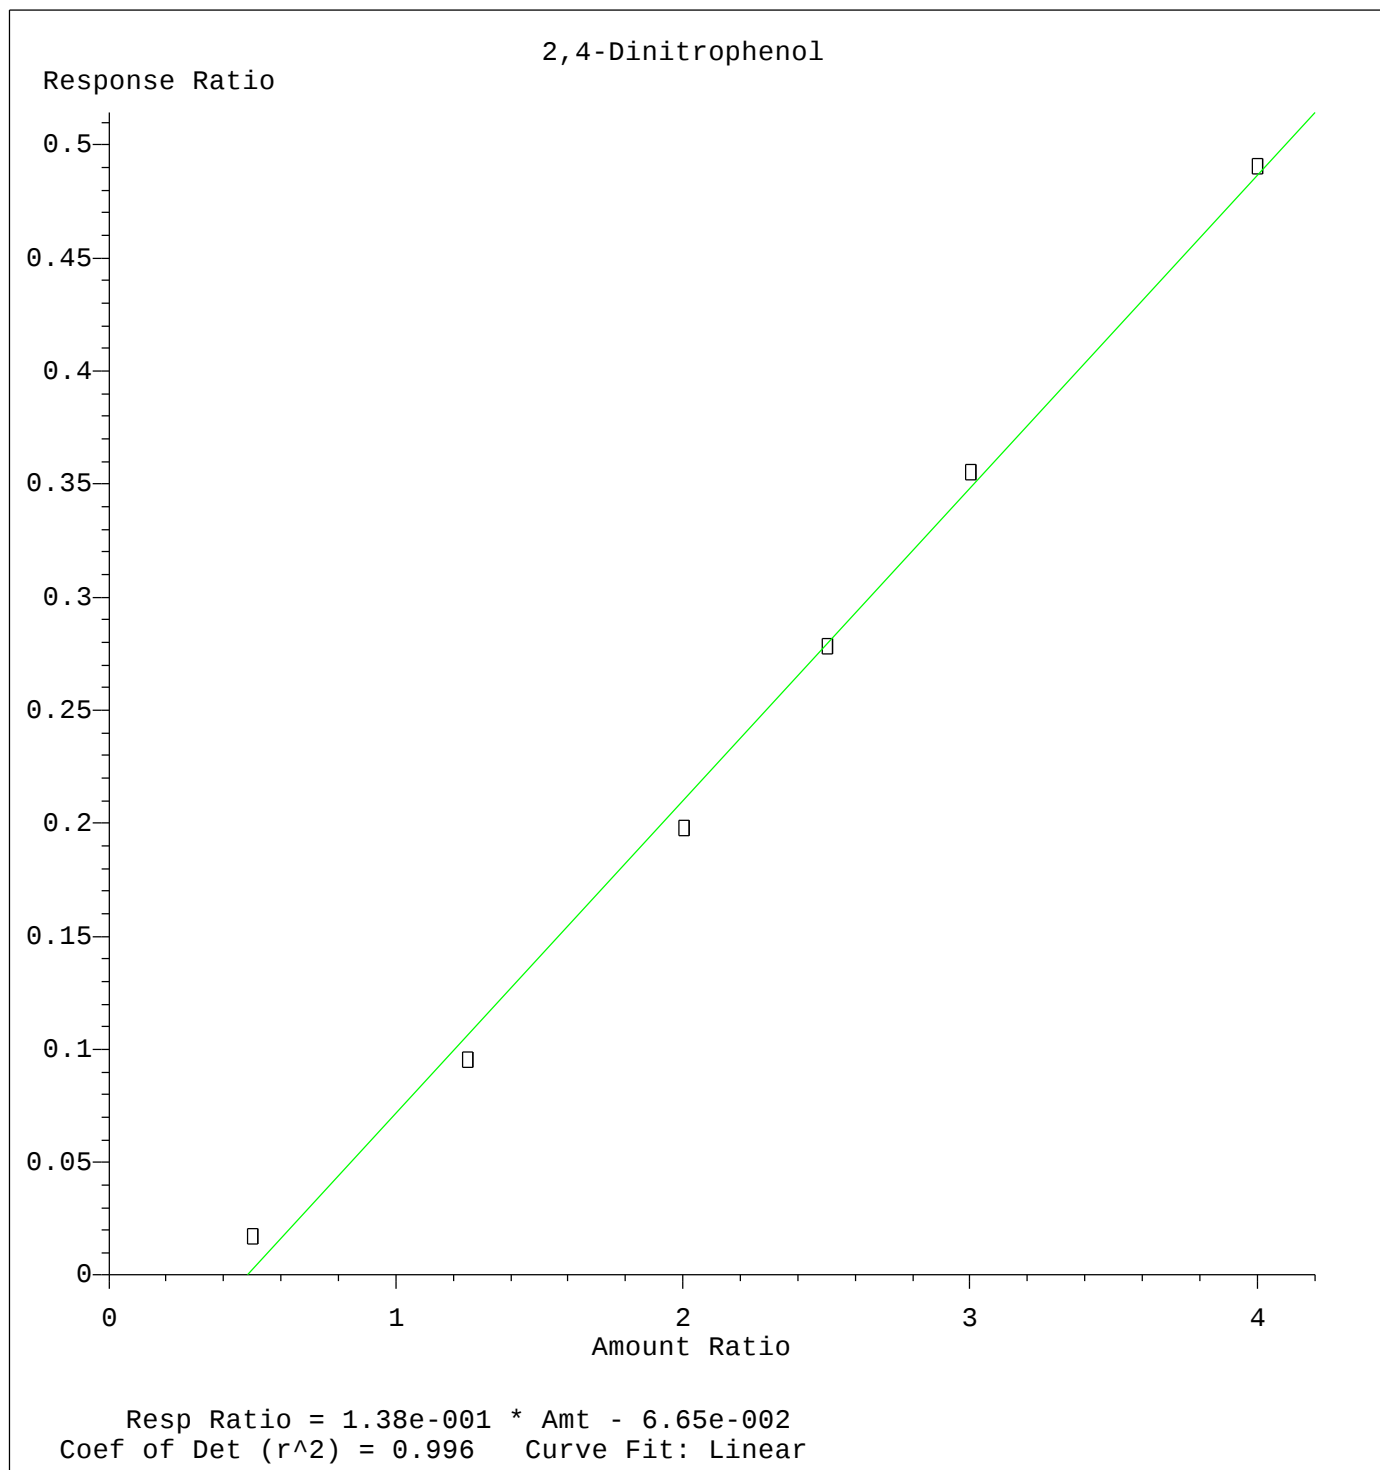

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
Calibration Table Last Updated: Fri Feb 23 02:43:46 2018

4,6-Dinitro-2-methylphenol

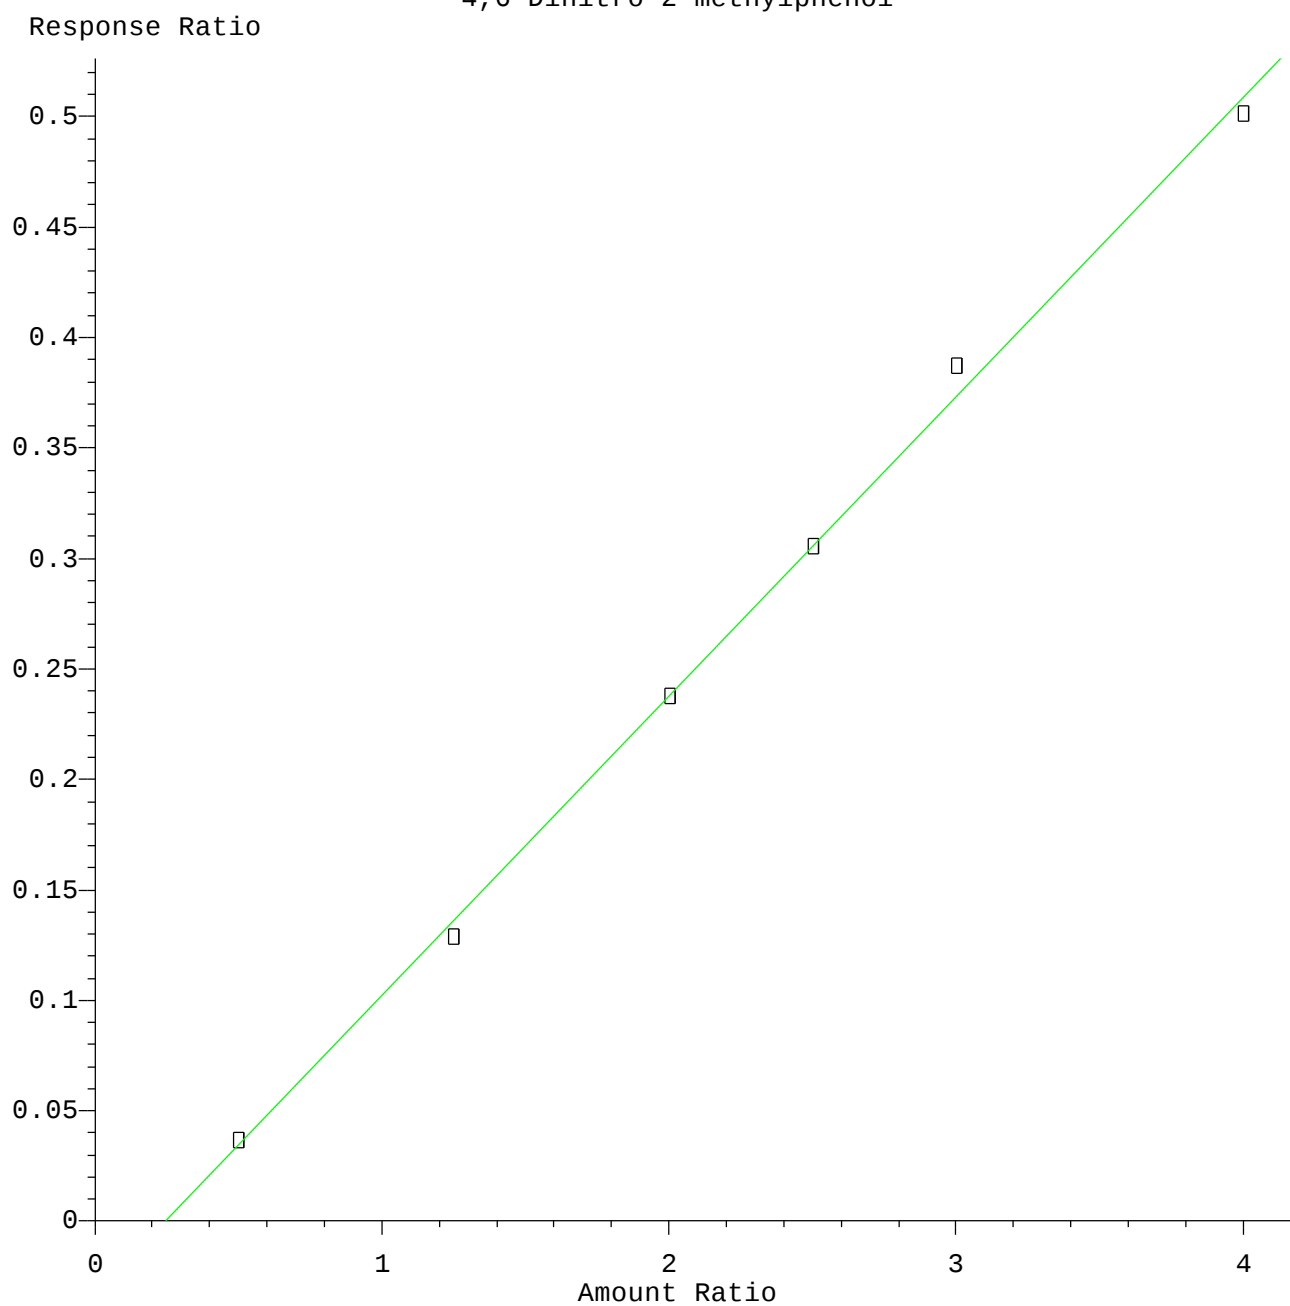


Resp Ratio = $1.36 \times 10^{-1} \times \text{Amt} - 3.35 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
Calibration Table Last Updated: Fri Feb 23 02:43:46 2018


2-Fluorobiphenyl

Response Ratio

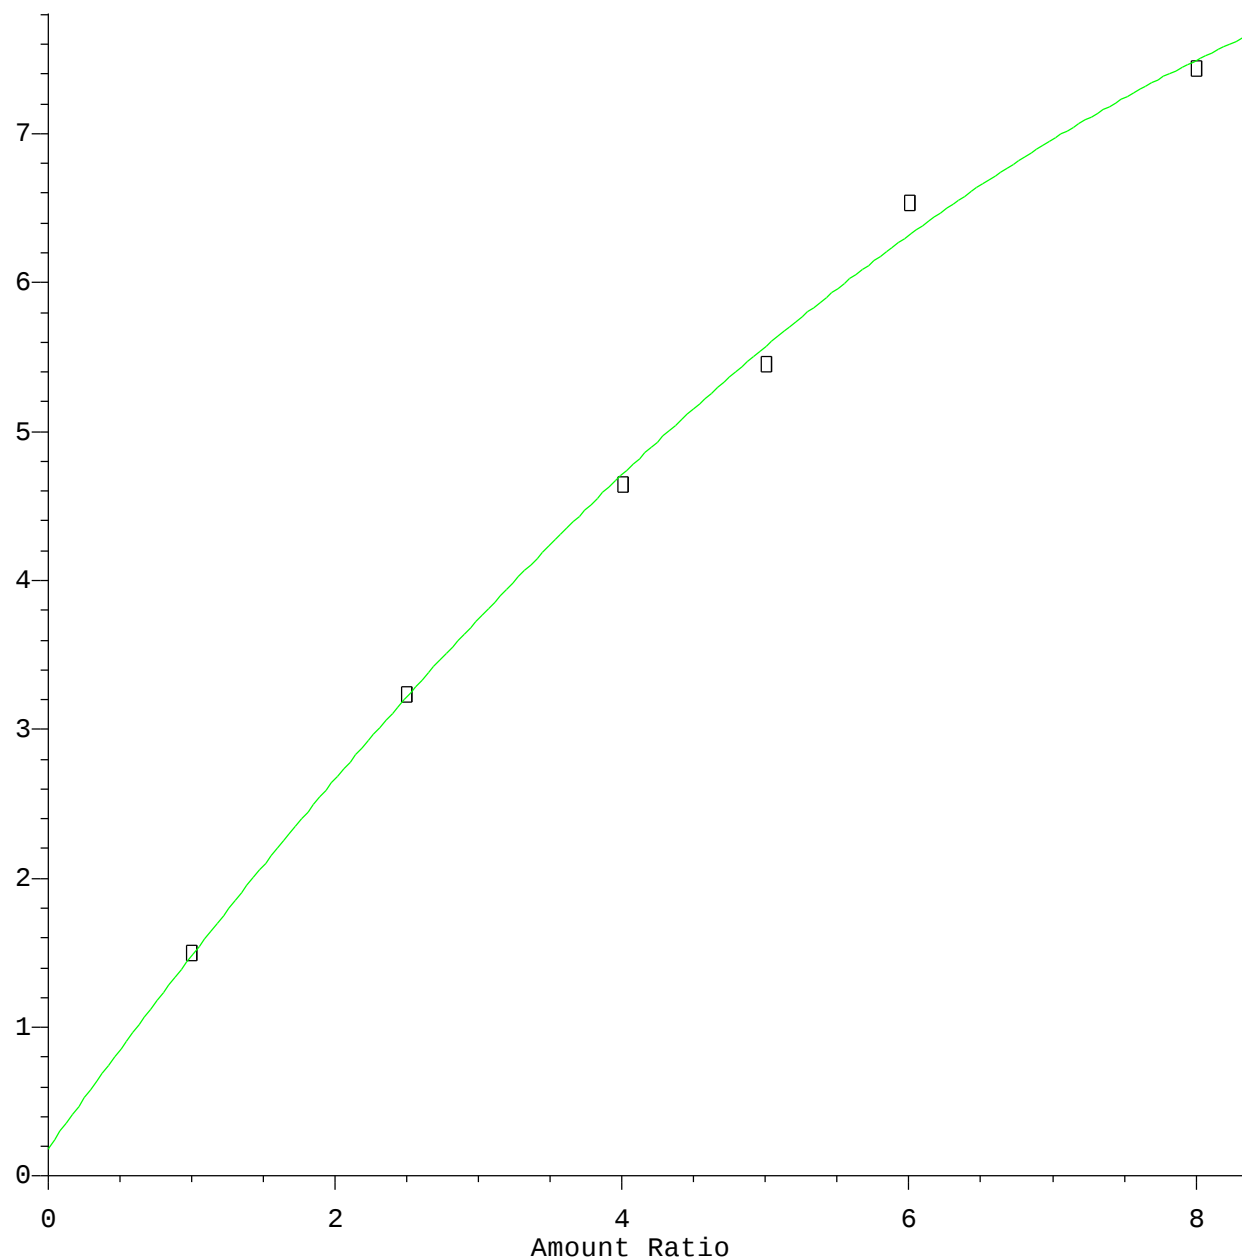

$R = -5.45e-002 A^2 + 1.35e+000 A + 1.85e-001$
Coef of Det (r^2) = 0.997 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
Calibration Table Last Updated: Fri Feb 23 02:43:46 2018

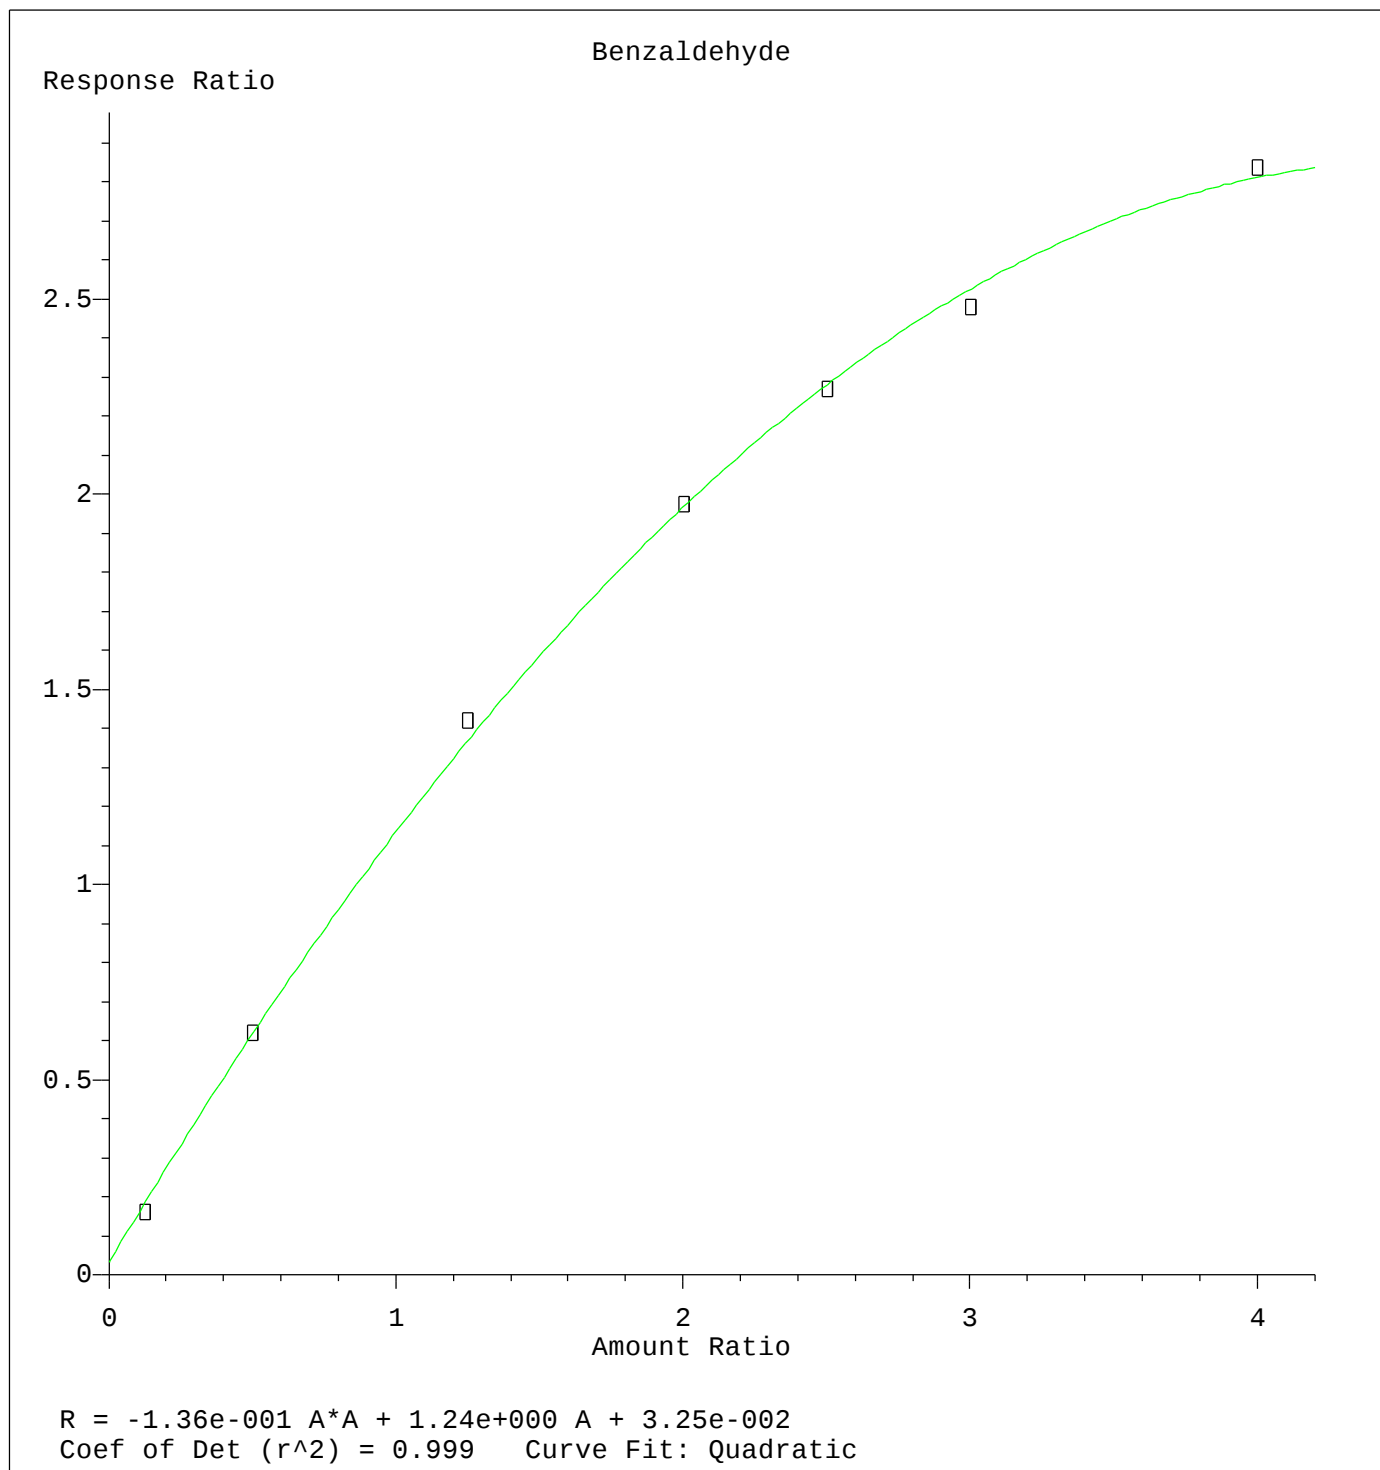

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
Calibration Table Last Updated: Fri Feb 23 02:43:46 2018