


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF022218\
 Data File : BF103153.D
 Acq On : 22 Feb 2018 11:07
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 23 02:43:46 2018

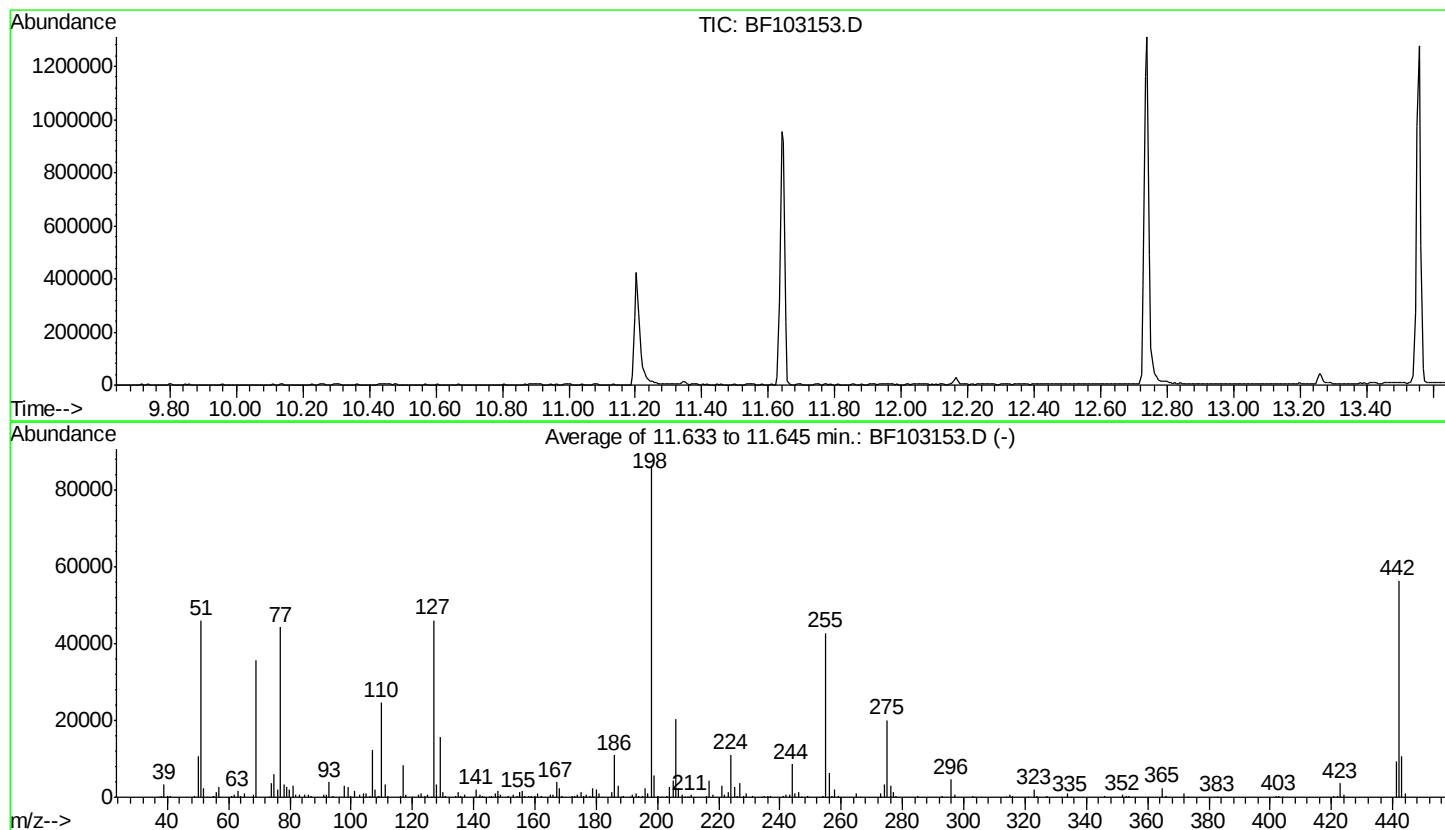

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.2	45984	PASS
68	69	0.00	2	1.5	535	PASS
69	198	0.00	100	41.3	35688	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.4	46152	PASS
197	198	0.00	2	1.1	927	PASS
198	198	100	100	100.0	86456	PASS
199	198	5	9	6.5	5628	PASS
275	198	10	60	23.2	20041	PASS
365	198	1	100	2.8	2453	PASS
441	443	0.01	100	85.3	9212	PASS
442	198	50	100	65.3	56444	PASS
443	442	15	24	19.1	10805	PASS