


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF022218\
 Data File : BF103162.D
 Acq On : 22 Feb 2018 15:12
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 23 02:43:46 2018

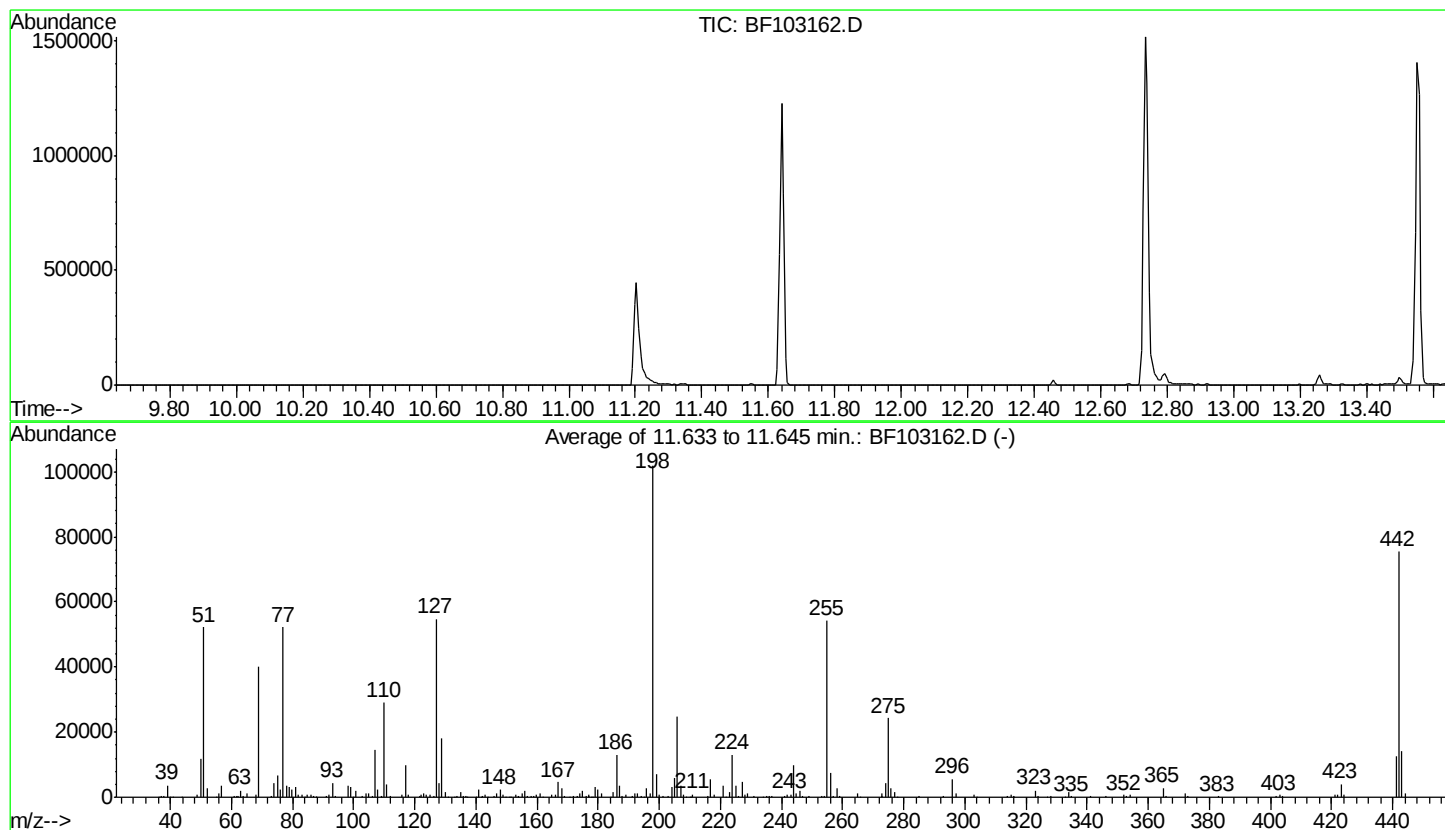

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.3	52272	PASS
68	69	0.00	2	1.6	642	PASS
69	198	0.00	100	39.2	39930	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.7	54672	PASS
197	198	0.00	2	1.0	1042	PASS
198	198	100	100	100.0	101853	PASS
199	198	5	9	7.1	7247	PASS
275	198	10	60	23.8	24246	PASS
365	198	1	100	2.8	2889	PASS
441	443	0.01	100	87.7	12474	PASS
442	198	50	100	74.0	75386	PASS
443	442	15	24	18.9	14218	PASS