
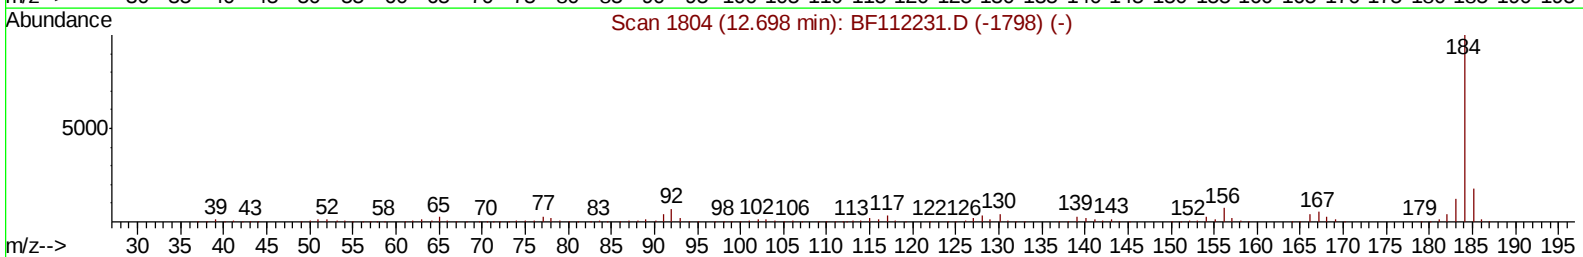
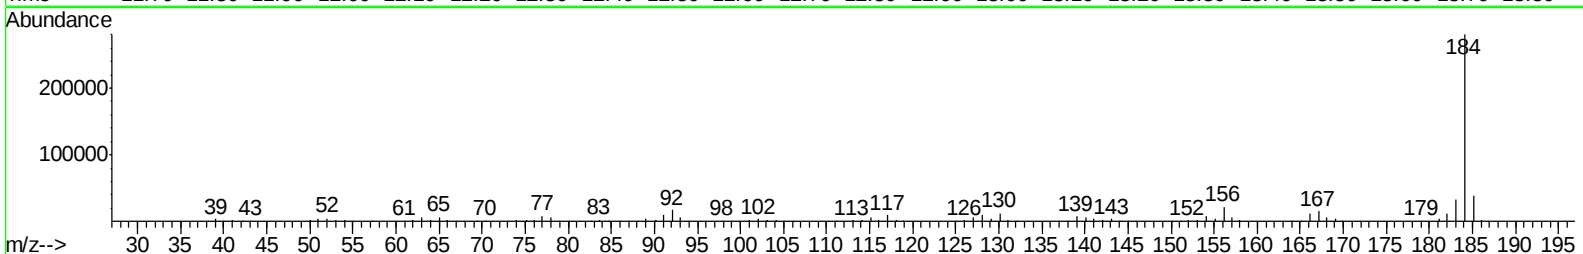


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF022219\  
Data File : BF112662.D  
Acq On : 22 Feb 2019 12:01  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 02:42:54 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF012519.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jan 28 10:38:18 2019  
Response via : Initial Calibration

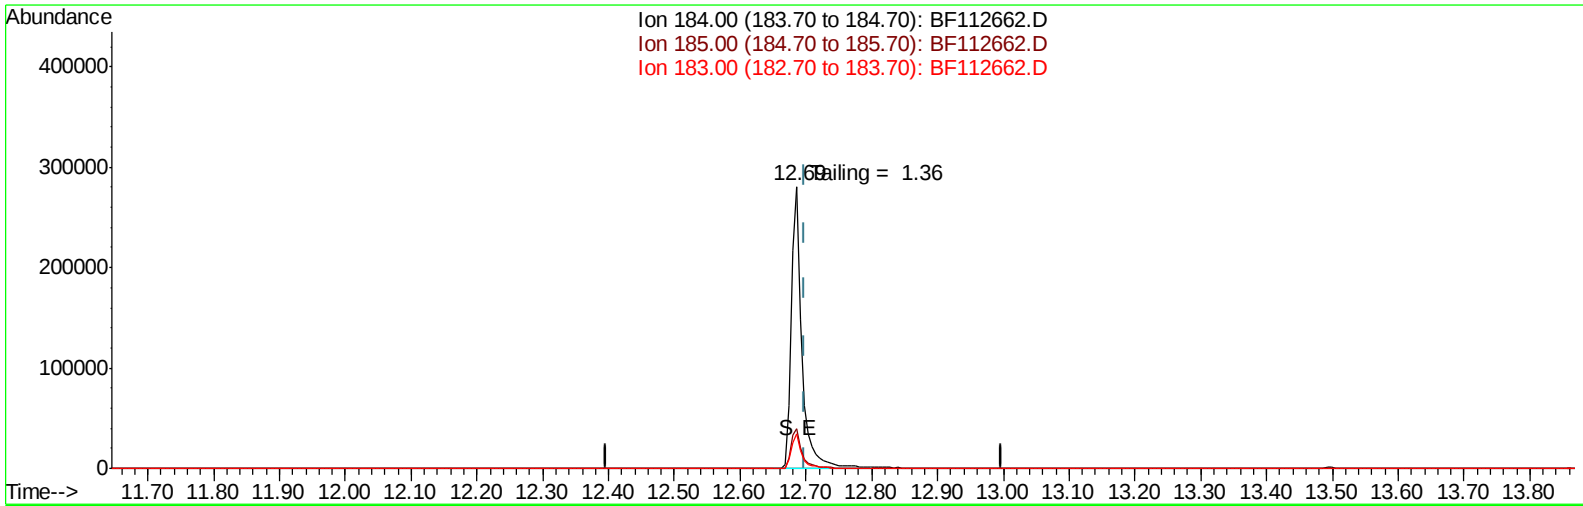

TIC: BF112662.D

(77) Benzidine




12.686min (-0.012) 0.00ng

response 318848

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 17.40 | 14.10 |
| 183.00 | 12.50 | 12.07 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF022219\  
Data File : BF112662.D  
Acq On : 22 Feb 2019 12:01  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 02:42:54 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF012519.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jan 28 10:38:18 2019  
Response via : Initial Calibration

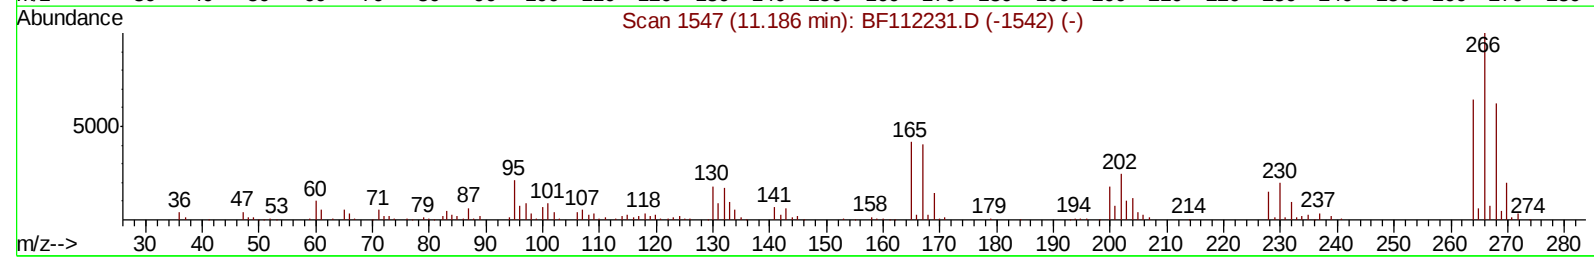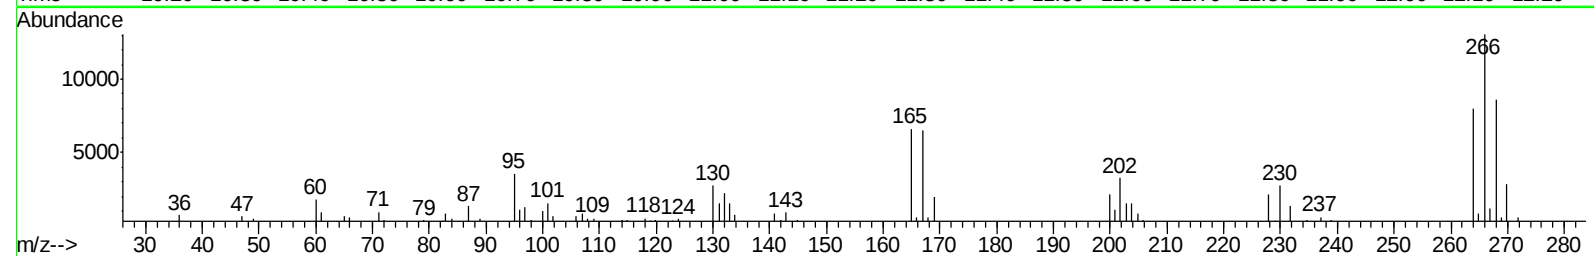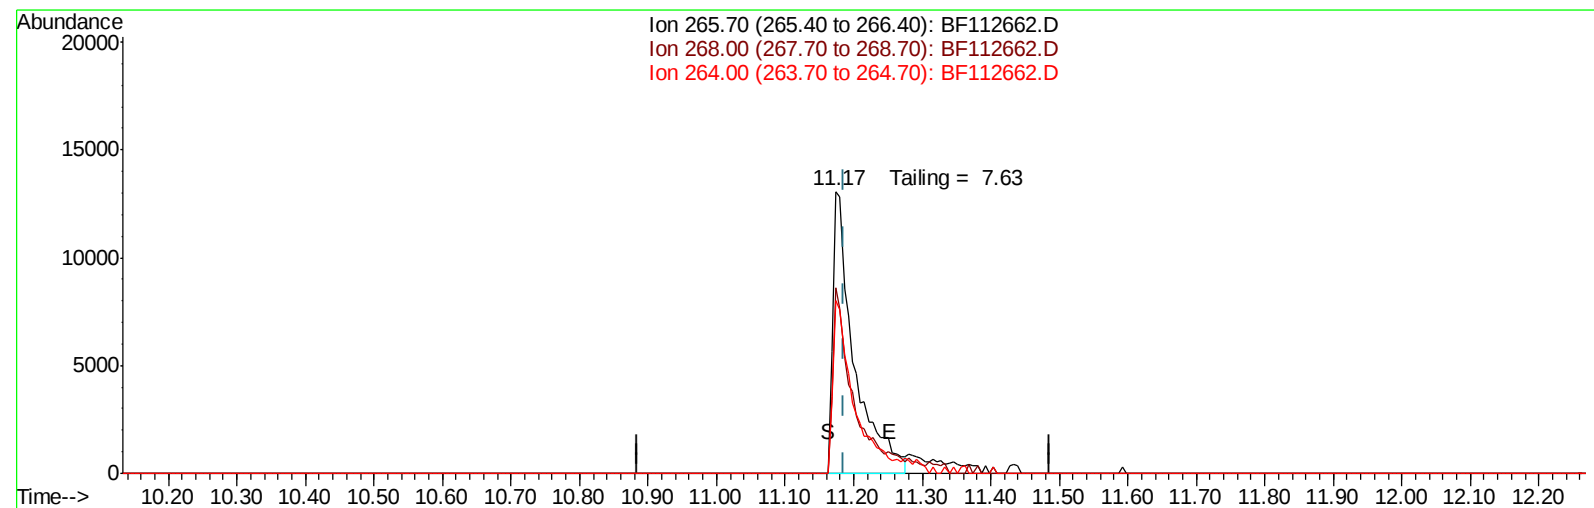

TIC: BF112662.D

(70) Pentachlorophenol (C)

11.175min (-0.012) 50972.31ng

response 27530

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 64.00 | 65.91 |
| 264.00 | 63.60 | 61.34 |
| 0.00   | 0.00  | 0.00  |